


A double-guidewire technique for endoscopic ultrasonography-guided pancreatic drainage after pancreaticoduodenectomy


OPEN
ACCESS

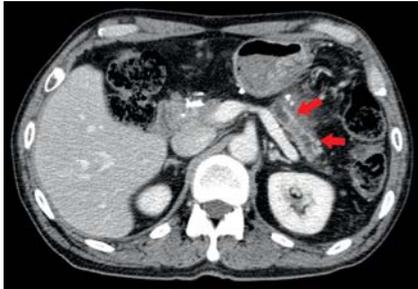


► **Fig. 1** Computed tomography revealing dilatation of the pancreatic duct (arrows) and obstruction of the pancreaticogastric anastomosis.

Endoscopic ultrasonography-guided pancreatic drainage (EUS-PD) is challenging owing to technical difficulties. The most important factor for these difficulties is the risk of guidewire dislodgement due to the short length of the guidewire, which can be left in the pancreatic duct (PD). The double-guidewire technique for EUS-guided hepaticogastrostomy has been shown to be effective to stabilize an endoscope and prevent guidewire dislodgement [1, 2]. Herein, we report that this technique is useful for EUS-PD.

A 71-year-old man underwent pancreaticoduodenectomy for intraductal papillary neoplasm 1 year prior to presentation at our hospital. Six months after the initial surgery, the tube that was placed through the pancreaticogastric anastomosis was dislodged. Diabetes mellitus was diagnosed with an increase of HbA1c from 5.7% to 7.0% in the following 3 months. Computed tomography imaging revealed dilatation of the PD and obstruction of the pancreaticogastric anastomosis (► **Fig. 1**). EUS-PD was performed to prevent the exacerbation of pancreatic function (► **Fig. 2**). The PD was punctured at the pancreaticogastric anastomosis using a 19-gauge needle, and a 0.025-inch hydrophilic guidewire was manipulated in the duct. A drill and balloon dilator were advanced to the fistula; however, a plastic stent could not be inserted be-

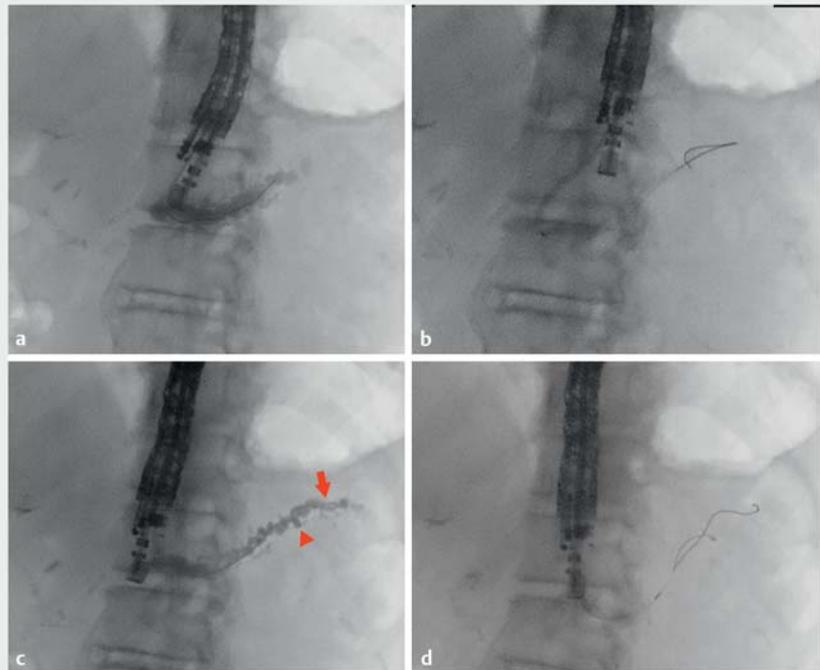

► **Fig. 2** **a** A guidewire was advanced to the dilated pancreatic duct after puncture of the pancreaticogastric anastomosis. **b** A plastic stent could not be advanced to the pancreatic duct since it was tortuous. **c** The second 0.035-inch guidewire (arrowhead) was placed using a double-lumen catheter. The placed 0.025-inch hard guidewire is shown (arrow). **d** The plastic stent on the 0.025-inch guidewire was advanced along with the 0.035-inch guidewire.

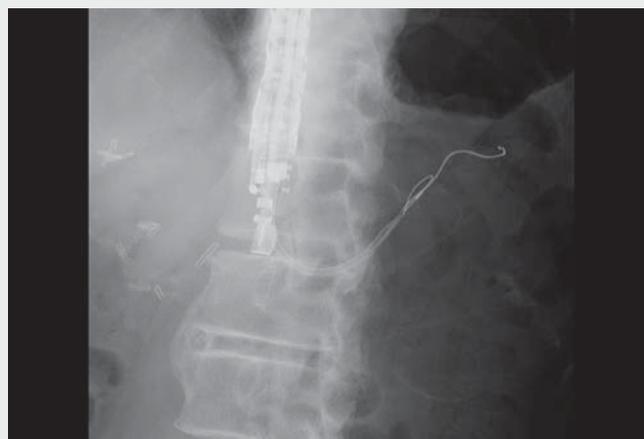

► **Video 1** A case wherein a double-guidewire technique for endoscopic ultrasonography-guided pancreatic drainage was effective in stabilizing the endoscope and preventing guidewire dislodgement.

cause the PD was tortuous and there was a risk of guidewire dislodgement. The original guidewire was changed to a 0.025-inch hard-type (Revowave Ultra-hard, Piolax Medical Devices, Inc., Kanagawa, Japan) through a double-lumen catheter, and a 0.035-inch guidewire (Jagwire Stiff Type, Boston Scientific, Marlborough, Massachusetts, USA) was additionally inserted into the PD. The scope could then be moved to advance the stent because the double-guidewire held the duct in place. Finally, a 7-Fr straight-type stent (Crane stent, SILUX Co., Ltd., Saitama, Japan) was placed across the anastomosis (► **Video 1**). The patient was discharged 4 days after PD stenting without any complications.

Endoscopy_UCTN_Code_TTT_1AS_2AD

Competing interests

The authors declare that they have no conflict of interest.

The authors

Shinichi Hashimoto  **Takuma Yamauchi, Takafumi Hamada, Issei Kojima, Makoto Hinokuchi, Shiroh Tanoue, Akio Ido**
Digestive and Lifestyle Diseases, Kagoshima University Graduate School of Medical and Dental Sciences, Kagoshima, Kagoshima, Japan

Corresponding author

Shinichi Hashimoto, MD
Digestive and Lifestyle Diseases, Kagoshima University Graduate School of Medical and Dental Sciences, 8-35-1 Sakuragaoka, Kagoshima 890-8520, Japan
Fax: +81-99-264-3504
kumdsh@m.kufm.kagoshima-u.ac.jp

References

- [1] Nakai Y, Oyama H, Kanai S et al. Double guidewire technique using an uneven double lumen catheter for endoscopic ultrasound-guided interventions. *Dig Dis Sci* 2021; 66: 1540–1547
- [2] Fujii Y, Kato H, Himei H et al. Double guidewire technique stabilization procedure for endoscopic ultrasound-guided hepaticogastrostomy involving modifying the guidewire angle at the insertion site. *Surg Endosc* 2022. doi:10.1007/s00464-022-09350-3

Bibliography

Endoscopy 2023; 55: E270–E271
DOI 10.1055/a-1974-9436
ISSN 0013-726X
published online 25.11.2022
© 2022. The Author(s).

This is an open access article published by Thieme under the terms of the Creative Commons Attribution-NonDerivative-NonCommercial License, permitting copying and reproduction so long as the original work is given appropriate credit. Contents may not be used for commercial purposes, or adapted, remixed, transformed or built upon. (<https://creativecommons.org/licenses/by-nc-nd/4.0/>)

Georg Thieme Verlag KG, Rüdigerstraße 14, 70469 Stuttgart, Germany



ENDOSCOPY E-VIDEOS

<https://eref.thieme.de/e-videos>



Endoscopy E-Videos is an open access online section, reporting on interesting cases and new techniques in gastroenterological endoscopy. All papers include a high quality video and all contributions are freely accessible online. Processing charges apply (currently EUR 375), discounts and waivers acc. to HINARI are available.

This section has its own submission website at <https://mc.manuscriptcentral.com/e-videos>