



A novel ultrathin cholangioscope for endoscopic ultrasound-guided antegrade intervention in patients with Roux-en-Y hepaticojejunostomy

OPEN
ACCESS

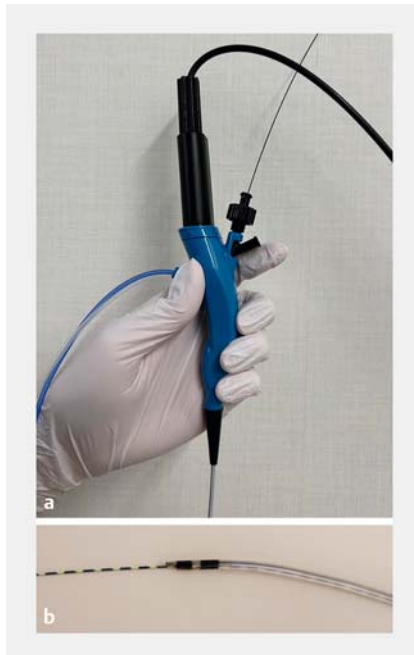

► Fig. 1 The novel ultrathin cholangioscope (**a,b**) is similar in size to a standard endoscopic retrograde cholangiopancreatography catheter. It has a 4.4-Fr tapered tip, a length of 1950 mm, and the compatible guidewire measures 0.025 inches. Independent water supply and suction channels are located 10 mm from the tip, so that simultaneous irrigation and observation can be performed, similarly to conventional large-diameter cholangioscopes.

Cholangitis can occur after biliary reconstructive surgery and is most commonly caused by hepaticojejunostomy anastomotic strictures and bile duct stones [1]. Endoscopic ultrasound-guided antegrade treatment (EUS-AG) has recently been performed in cases where balloon enteroscopy-assisted endoscopic retrograde cholangiopancreatography (BE-ERCP) is difficult [2]. In EUS-AG, cholangioscopy is needed to obtain direct visual information on the anastomosis. However, it is often difficult to insert a cholangioscope in a significantly dilated fistula

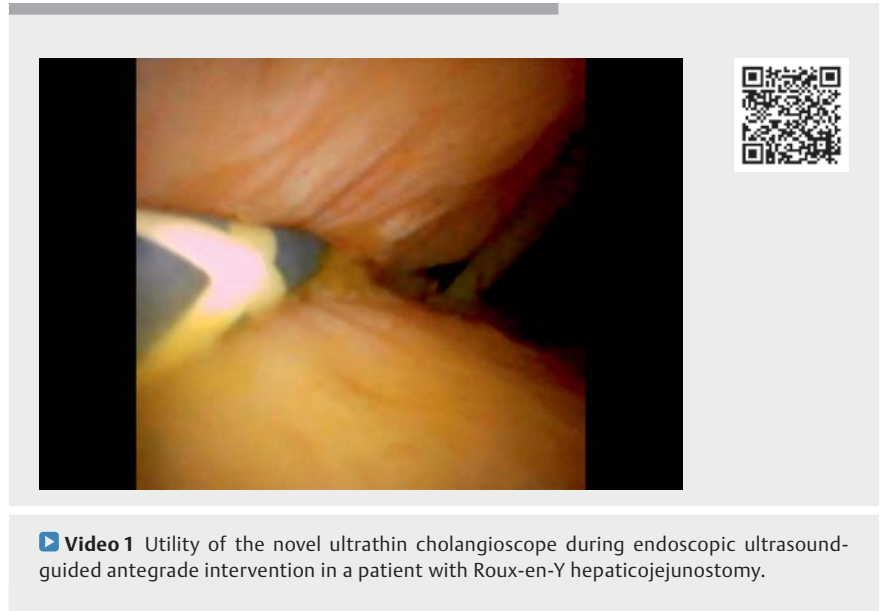

► Video 1 Utility of the novel ultrathin cholangioscope during endoscopic ultrasound-guided antegrade intervention in a patient with Roux-en-Y hepaticojejunostomy.

due to the narrowness of the intrahepatic bile ducts. We report the feasibility of a novel ultrathin cholangioscope (DRES Slim Scope; Japan Lifeline Co., Ltd., Tokyo, Japan) that has almost the same diameter as a standard ERCP catheter (**► Fig. 1**).

An 80-year-old man who underwent hepaticojejunostomy with Roux-en-Y reconstruction for cholangiocarcinoma developed cholangitis with intrahepatic bile duct dilation. BE-ERCP was initially performed for biliary drainage and evaluation of the hepaticojejunostomy anastomosis, but the scope failed to reach the anastomosis site. Therefore, we converted to an EUS-guided hepaticogastrostomy and placed a 7-Fr single-pigtail plastic stent from the intrahepatic duct to the stomach. Cholangitis rapidly improved, and no adverse events were noted.

A standard duodenoscope was inserted 2 weeks postoperatively, followed by guidewire insertion from the fistula into the bile duct, alongside the hepaticogastrostomy stent. Subsequently, the stent


was removed, and the ultrathin cholangioscope was inserted without any fistula dilation. No stricture was observed at the anastomosis site, and there was no evidence of recurrence. Therefore, balloon cleaning was only performed antegradely without replacement of the stent (**► Fig. 2**, **► Video 1**). The treatment achieved good clinical course with no adverse outcomes.

Although the novel ultrathin cholangioscope does not have a large working channel, its small diameter allows easy insertion and manipulation, and it is less invasive and inexpensive. EUS-AG can be considered a good indication for this novel device.

Endoscopy_UCTN_Code_TTT_1AS_2AD


Competing interests

T. Inoue has received honoraria from Japan Lifeline Co., Ltd, unrelated to the submitted work. R. Kitano, M. Ibusuki, Y. Kobayashi, K. Ito, and M. Yoneda declare that they have no conflict of interest.

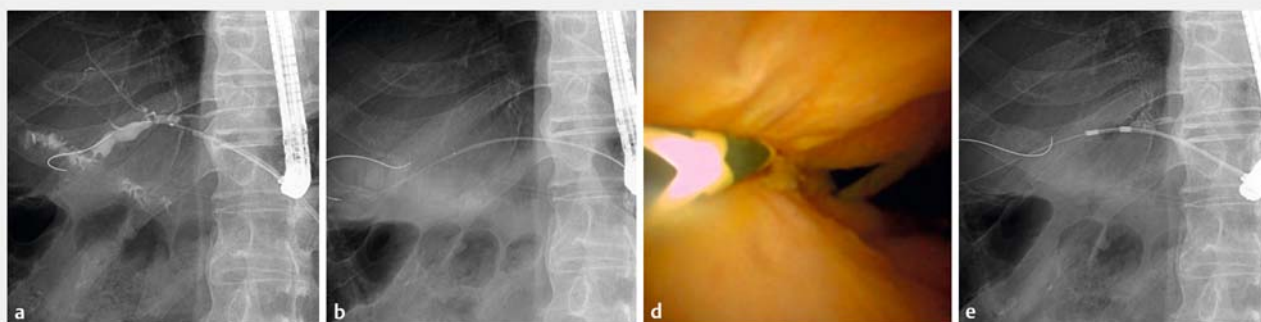

► **Fig. 2** Use of the ultrathin cholangioscope. **a** A 0.025-inch guidewire was inserted into the bile duct, from the fistula, alongside the hepaticogastrostomy stent. **b** Subsequently, the stent was removed, and the ultrathin cholangioscope was inserted without any fistula dilation. **c** No stricture was observed at the anastomosis site, and there was no evidence of recurrence. **d** Therefore, balloon cleaning was only performed antegradely without replacing the stent.

The authors

Tadahisa Inoue , **Rena Kitano**, **Mayu Ibusuki**,
Yuji Kobayashi, **Kiyoaki Ito**, **Masashi Yoneda**
Department of Gastroenterology, Aichi Medical
University, Nagakute, Japan

Corresponding author

Tadahisa Inoue, MD, PhD, FJGES
Department of Gastroenterology, Aichi
Medical University, 1-1 Yazakokarimata,
Nagakute, Aichi 480-1195, Japan
tinoue-tag@umin.ac.jp

References

- [1] Dimou FM, Adhikari D, Mehta HB et al. Incidence of hepaticojunostomy stricture after hepaticojunostomy. *Surgery* 2016; 160: 691–698

- [2] Homma T, Yamamoto K, Tsuchiya T et al. A case of severe hepatolithiasis after hepaticojunostomy with Roux-en-Y reconstruction treated by endoscopic ultrasound-guided transhepatic antegrade stone removal. *Endoscopy* 2021; 53: E230–E231. Correction in *Endoscopy* 2021; 53: C7

Bibliography

Endoscopy 2023; 55: E953–E954

DOI 10.1055/a-2127-4957

ISSN 0013-726X

© 2023. The Author(s).

This is an open access article published by Thieme under the terms of the Creative Commons Attribution License, permitting unrestricted use, distribution, and reproduction so long as the original work is properly cited.

(<https://creativecommons.org/licenses/by/4.0/>)

Georg Thieme Verlag KG, Rüdigerstraße 14,
70469 Stuttgart, Germany



ENDOSCOPY E-VIDEOS

<https://eref.thieme.de/e-videos>



E-Videos is an open access online section of the journal *Endoscopy*, reporting on interesting cases

and new techniques in gastroenterological endoscopy. All papers include a high-quality video and are published with a Creative Commons CC-BY license. *Endoscopy E-Videos* qualify for HINARI discounts and waivers and eligibility is automatically checked during the submission process. We grant 100% waivers to articles whose corresponding authors are based in Group A countries and 50% waivers to those who are based in Group B countries as classified by Research4Life (see: <https://www.research4life.org/access/eligibility/>).

This section has its own submission website at
<https://mc.manuscriptcentral.com/e-videos>