

Effect of dry cryogenic treatment on Vickers hardness and wear resistance of new martensitic shape memory nickel-titanium alloy

Thilla Sekar Vinothkumar¹, Deivanayagam Kandaswamy¹, Gopalakrishnan Prabhakaran²,
Arunachalam Rajadurai³

Correspondence: Dr. Thilla Sekar Vinothkumar
Email: vinothkumar_ts@yahoo.com

¹Department of Conservative Dentistry and Endodontics, Faculty of Dental Sciences of Sri Ramachandra University, Chennai, Tamil Nadu, India,
²Department of Mechanical Engineering, Velammal Engineering College, Chennai, Tamil Nadu, India,
³Department of Production Technology, MIT Campus, Anna University, Chennai, Tamil Nadu, India

ABSTRACT

Objectives: The aim of this study is to investigate the role of dry cryogenic treatment (CT) temperature and time on the Vickers hardness and wear resistance of new martensitic shape memory (SM) nickel-titanium (NiTi) alloy. The null hypothesis tested was that there is no difference in Vickers hardness and wear resistance between SM NiTi alloys following CT under two soaking temperatures and times. **Materials and Methods:** The composition and the phase transformation behavior of the alloy were examined by X-ray energy dispersive spectroscopy and differential scanning calorimetry, respectively. Fifteen cylindrical specimens and 50 sheet specimens were subjected to different CT conditions: Deep cryogenic treatment (DCT) 24 group: -185°C , 24 h; DCT six group: -185°C , 6 h; shallow cryogenic treatment (SCT) 24 group: -80°C , 24 h; SCT six group: -80°C , 6 h; and control group. Wear resistance was assessed from weight loss before and after reciprocatory wet sliding wear. **Results:** The as-received SM NiTi alloy contained 50.8 wt% nickel and possessed austenite finish temperature (A_f) of 45.76°C . Reduction in Vickers hardness of specimens in DCT 24 group was highly significant ($P < 0.01$; Tukey's honest significant difference [HSD]). The weight loss was significantly higher in DCT 24 group ($P < 0.05$; Tukey's HSD). **Conclusion:** Deep dry CT with 24 h soaking period significantly reduces the hardness and wear resistance of SM NiTi alloy.

Key words: Cryogenic treatment, nickel-titanium, shape memory, Vickers hardness, wear resistance

INTRODUCTION

The nickel-titanium (NiTi) alloy, which is used in the manufacturing of rotary endodontic instruments, is an exotic metal that can be subjected to thermomechanical treatment in order to alter shape memory (SM) and superelasticity.^[1] Although NiTi alloys possess these unique properties, fracture of rotary instruments in the canal without warning is unavoidable when compared with stainless steel.^[2] To overcome this difficulty, either new alloys could be used or the manufacturing process (machining or twisting) could be altered.^[3,4]

There is a significant improvement in the design and control of raw NiTi alloy over the last decade

in relation to manufacturing process and material properties.^[3,5-8] Based on the characterization experiments performed earlier, the martensitic SM NiTi alloys possess significant proportion of stable martensite phase at working temperature that is

This is an open access article distributed under the terms of the Creative Commons Attribution-NonCommercial-ShareAlike 3.0 License, which allows others to remix, tweak, and build upon the work non-commercially, as long as the author is credited and the new creations are licensed under the identical terms.

For reprints contact: reprints@medknow.com

How to cite this article: Vinothkumar TS, Kandaswamy D, Prabhakaran G, Rajadurai A. Effect of dry cryogenic treatment on Vickers hardness and wear resistance of new martensitic shape memory nickel-titanium alloy. Eur J Dent 2015;9:513-7.

DOI: 10.4103/1305-7456.172626

the body temperature.^[5] Consequently, martensitic instruments deform easily and regain their original shape when heated above the transformation temperature during sterilization.^[9] They possess active austenite finish temperature (A_f) of -55°C , and the superelastic (SE) property exists 50°C above the A_f temperature that is 105°C .^[10] Despite the extreme flexibility, canal centering ability, and superior canal tracking,^[9,10] these alloys do not possess the conventional stress-induced martensitic transformation as observed in SE NiTi alloys.^[11]

The major drawback of martensitic instruments is their permanent plastic deformation following instrumentation.^[12] Peters *et al.* reported that 82% of the SM rotary instruments plastically deformed postinstrumentation, of which 37% of the instruments did not recover their shape after sterilization.^[12] Also, smaller SM instruments have a larger tendency to plastically deform than larger instruments for a given torque. Therefore, the operator should be cautious while reusing small rotary instruments.^[13]

Cryogenic treatment (CT) is an inexpensive, one-time treatment of subjecting metals to very low temperatures that affects the entire core components rather the surface alone.^[14,15] Based on the soaking temperature, the CT can be shallow (-80°C ; shallow cryogenic treatment [SCT])^[16] or deep (-185 to -196°C deep cryogenic treatment [DCT]).^[17,18] Based on the contact of specimens with liquid nitrogen, the process may be dry (not immersed) or wet (immersed).^[19] CT of rotary endodontic instruments made up of SE NiTi alloy has shown increased cutting efficiency^[19] and microhardness.^[20] Improvement in steel tool life of 200% following CT has been reported due to phase transformation of retained austenite to martensite as well as to the deposition of fine carbide particles.^[18,21] Both stainless steel^[20] and SM NiTi alloys^[10] have A_f temperature above the body temperature. However, the effect of CT on the mechanical properties of SM NiTi alloys remains unclear. Therefore, the purpose of this preliminary study is to evaluate the effect of dry CT temperature and time on the hardness and wear resistance of SM NiTi alloys. The null hypotheses tested were as follows:

- There are no differences in Vickers hardness and wear resistance between SM NiTi alloys following DCT and SCT (CT temperature)
- There are no differences in Vickers hardness and wear resistance between SM NiTi alloys following exposure to 6 h and 24 h (CT time).

MATERIALS AND METHODS

Raw SM NiTi alloy in the form of sheet and rod from the same ingot was obtained for the investigation.^[22] The elemental composition was determined for the SM alloy using scanning electron microscope (CX-200; Coxem Ltd., Daejeon, South Korea) coupled to energy dispersive X-ray spectrometer.

The transformation temperature range was determined using differential scanning calorimetry (DSC). A small piece of alloy (10–12 mg) was cut using water-cooled, slow-speed diamond saw to avoid changes in the transformation temperature range. The phase transformation was monitored using a differential scanning calorimeter (DSC 204; Netzsch-Geratebau GmbH, Germany) over a temperature range from -70°C to 100°C . Cooling DSC curve was obtained by first heating the specimen from room temperature to 100°C and then cooled to -70°C . Heating DSC curve was obtained by subsequently heating the specimen to 100°C . The austenite starting and finishing temperature and martensite starting and finishing temperature were identified from the DSC curve in order to confirm the transformation temperature range of SM alloy.

X-ray diffraction (XRD) was performed on a specimen after polishing to identify the phases. The analysis was performed at room temperature on an X-ray diffractometer (MiniFlex II-C, Rigaku, Tokyo, Japan). The angular 2θ diffraction range was 10 – 100° at 0.02° steps and 2 s of step time. The XRD system was operated with Cu-K α anode ($\lambda = 1.5406 \text{ \AA}$) with 40 kV accelerating voltage and 40 mA beam current. A silicon standard (640b Silicon Powder XRD Spacing, Standard Reference Material; NIST, Gaithersburg, MD, USA) was used to calibrate the diffractometer. The International Centre for Diffraction Data (ICDD) database (PDF release 2004; ICDD, Newton Square, PA) was used to identify the austenite and martensite phase peak.

Cryogenic process

Fifteen cylindrical specimens (10 mm height and 9 mm diameter) and 50 sheet specimens (15 mm \times 15 mm square) were sectioned from the as-received NiTi sheet and rod with the help of wire electrical discharge machine (AQ300L; Sodick, Shaumburg, IL). The dry CT facility used in the present study has been utilized in the previous study.^[19] Both cylindrical and sheet specimens were randomly divided into five groups of three and 10

each, respectively. The groups were categorized based on the soaking temperature and time as follows: DCT 24 group: -185°C , 24 h; DCT six group: -185°C , 6 h; SCT 24 group: -80°C , 24 h; SCT six group: -80°C , 6 h; and Control (Ctrl) group: No treatment. The cooling rate of $1^{\circ}\text{C}/\text{min}$ (3 h) and warming rate $0.6^{\circ}\text{C}/\text{min}$ (6 h) were kept constant for all experimental groups.

Vickers hardness

All cylindrical specimens (3/group) were mounted and the cut surface was ground and polished with sandpaper (Carbimet Paper Discs, Buehler: 240 and 600 grit) in a polishing machine (Bainpol, Chennai Metco Pvt Ltd, Chennai, India). Final polishing was done with alumina paste (Alpha Micropolish, Buehler: 6 μm , 1 μm and 0.5 μm particle sizes). Hardness measurements were performed in each specimen with Vicker's hardness tester (VM-50, Fuel Instruments and Engineers Pvt. Ltd., Kohlapur, India) at room temperature with 5 kg load and 15 s dwell time. Five indentations were made in each specimen with a square-based pyramidal diamond indenter at the center and at equidistant adjacent locations in each specimen ($n = 15$). The two diagonals of the indentations were measured to the nearest 0.1 μm with a filar micrometer and averaged. Hardness was taken as the maximum force divided by the area of contact.

Wear resistance

Fifty NiTi sheet specimens (10/group) were subjected to reciprocal sliding wear. Wear test was conducted on a reciprocatory friction and wear monitor as per the American Society for Testing and Materials standards.^[23] The reciprocating speed was adjusted to 10 Hz with a stroke length of 10 mm and duration of 4 h with the

vertical load of 10 N. The En-31 steel was selected as opposing material during reciprocating sliding wear in order to have higher hardness than that of NiTi alloy.^[24] Physiological saline solution was used as coolant during the experiment. The SM NiTi specimens were weighed in an electronic weigh balance (Analytical Plus; Ohaus Corporation, Pine Brook, NJ) before and after the sliding test and their wear resistance were quantified by calculating the loss of weight.^[25]

The significance for hardness and weight loss data was analyzed using one-way ANOVA followed by *post-hoc* multiple comparisons using Tukey's honest significant difference (HSD) test. Statistical analysis was performed using SPSS software version 16.0 (SPSS Inc. Chicago, IL) at a 0.05 significance level.

RESULTS

The elemental composition of the as-received SM alloy was nickel rich (nickel – 50.8 wt%; titanium – 48.4 wt%) with trace elements. The typical DSC curve of the raw material exhibited single well-defined peak on heating and two peaks on cooling [Figure 1]. The A_f temperature was found to be 45.76°C that is well above the body temperature. XRD pattern confirmed the presence of martensite phase at room temperature [Figure 2].

The Vickers hardness number (VHN) of specimens in all groups was above 200 VHN [Table 1]. The specimens in DCT 24 exhibited the least hardness (212 VHN) whereas the specimens in Ctrl showed the maximum value (238 VHN). The statistical difference in VHN of different groups was highly significant ($P < 0.01$; one-way ANOVA). The mean VHN of Ctrl was significantly higher than that of DCT 24 and

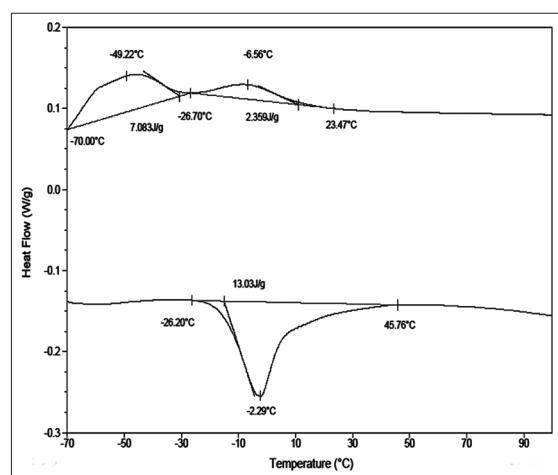


Figure 1: Differential scanning calorimetry curve of the specimen of the as-received nickel-titanium shape memory alloy

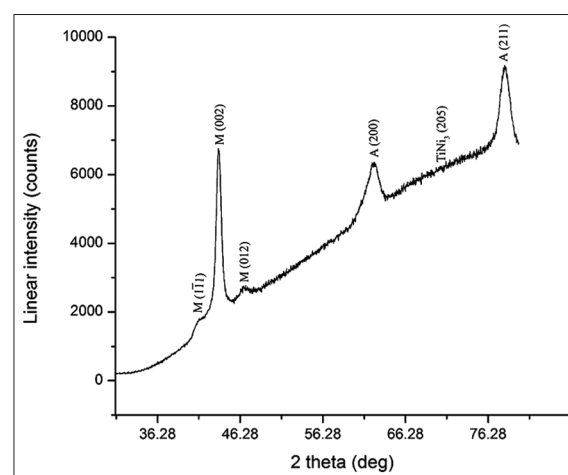


Figure 2: X-ray diffraction pattern of the as-received specimen at room temperature

Table 1: Inter-group comparison of the Vickers hardness values ($n=15$) from cylindrical specimens and weight loss values ($n=10$) from sheet specimens

| | Vickers hardness [†] (VHN) | Weight loss [†] ($\times 10^{-3}$ g) |
|--------|-------------------------------------|------------------------------------------------|
| DCT 24 | 212.27 \pm 4.85 ^a | 4.67 \pm 0.01 ^d |
| DCT 6 | 225.60 \pm 8.60 ^b | 4.51 \pm 0.03 ^e |
| SCT 24 | 234.27 \pm 15.05 ^c | 3.47 \pm 0.06 ^f |
| SCT 6 | 237.33 \pm 8.47 ^c | 3.57 \pm 0.04 ^g |
| Ctrl | 238.33 \pm 11.26 ^c | 2.94 \pm 0.03 ^h |

[†]One-way ANOVA and Tukey's *post-hoc* test. Data are expressed as mean \pm SD. Values with different superscript letters indicate a self explanatory for significant difference between the groups ($P < 0.05$). SD: Standard deviation, VHN: Vickers hardness number, DCT: Deep cryogenic treatment, SCT: Shallow cryogenic treatment, Ctrl: Control

DCT 6 ($P < 0.05$; Tukey's HSD). The mean difference in VHN of DCT specimens treated with 24 h and 6 h soaking period was highly significant ($P < 0.01$) in contrast to that of SCT specimen ($P > 0.05$).

The difference in mean weight loss following wet sliding wear in different groups [Table 1] was statistically significant ($P < 0.01$; one-way ANOVA). The mean weight loss in all the experimental groups was significantly ($P < 0.01$; Tukey's HSD) higher than that of Ctrl. The mean difference in weight loss of specimens treated with 24 h and 6 h soaking period was highly significant ($P < 0.01$; Tukey's HSD) in both DCT and SCT specimens.

DISCUSSION

CT of alloys during manufacturing has been successful in improving their hardness and wear resistance.^[14,21,26] Although SM alloys are extremely flexible with longer fatigue life due to the presence of martensite phase at working temperature,^[27] supplementary CT would further increase the volume of martensite^[14] resulting in superadded benefits. The objective of this study is only to assess the effect of soaking temperature and time. Hence, the cooling rate and warming rate were maintained constant. The results of this study showed a significant difference in Vickers hardness and wear resistance of SM NiTi alloys between those treated with DCT and SCT. Therefore, the first null hypothesis was rejected. However, the soaking time had a significant influence on the properties of the SM NiTi alloy pertaining to DCT. Thus, the second null hypothesis was partially rejected.

The results of this study showed that the composition and transformation temperature range were closely approximating with that of the commercial SM files.^[3] Nevertheless, the mechanical properties are more sensitive to the transformation temperature

range rather than the composition.^[1] The phase transformations were more prominent with a single stage (martensite \rightarrow austenite) while heating and two stage (austenite \rightarrow R-phase \rightarrow martensite) while cooling.^[3,28] Raw materials were selected prior to manufacturing for two reasons – To avoid the influence of manufacturing methods (machining/twisting) and thermomechanical processing on NiTi properties and the dimension of the specimens were customized according to the test requirements.

Hardness tests were performed on polished surfaces to ensure low surface roughness that might lead to errors in depth calculations. The average microhardness values of M-wire SM NiTi alloy, controlled memory SM NiTi alloy, conventional SE NiTi alloy, and fully annealed NiTi alloy were 390 VHN, 315 VHN, 353 VHN, and 200 VHN, respectively.^[6,29,30] However, the as-received specimens in this study exhibited mean hardness of 238 VHN as a result of cold working. When compared with the Ctrl group, there is a significant reduction in hardness value of the specimens in the DCT groups. In the SCT groups, significant reduction in hardness of specimens was appreciated neither between them nor with the Ctrl. The reduction in hardness of the specimens following DCT could be speculated to the complete transformation of retained austenite into martensite phase.^[18] Microstructural characterization of the same alloy performed earlier using optical microscope, scanning electron microscope, and XRD has confirmed the reduction in volume of austenite and increase in martensite.^[31] This highlights the importance of deep dry CT in a controlled manner, which avoids the thermal shock as observed in wet CT.^[19] In contrast, deep wet CT increased the microhardness of SE NiTi instruments.^[20]

The weight loss data of the specimens in the experimental groups showed a relatively higher value in DCT 24 suggesting its poor wear resistance. This could be correlated with the reduction in hardness and increase in martensite content of the specimens.^[24] The wear resistance of the martensite phase is relatively lower than the austenite phase as they undergo plastic deformation due to their low strength.^[32]

The soaking period plays an important role in significantly altering the hardness of SM NiTi specimens as far as DCT is concerned. Longer soaking time of 24 h yielded favorable results by providing adequate time for the transformation of retained austenite to martensite phase. The SM NiTi alloys show remarkable fatigue resistance and flexibility due to the presence of proportionately higher martensite phase.^[4]

Accordingly, the hardness is reduced resulting in a decrease in likelihood of instrument fracture during use.^[33] However, the wear resistance was significantly affected in both DCT and SCT group between 24 h and 6 h soaking period.

CONCLUSION

Dry CT appears to be a promising supplementary method in the manufacturing of SM NiTi endodontic instruments. Under the given experimental framework, deep dry CT with 24 h soaking period significantly reduces the hardness and wear resistance of SM NiTi alloy. Further investigation is required to evaluate the impact of CT on cutting efficiency and fatigue life of the instruments made out of this new SM alloy.

Acknowledgment

This work was carried out as part of first author's Ph.D program and was partly supported by "Young Research Faculty Grant" provided by Sri Ramachandra University, India. The authors deny any other conflict of interest related to this study.

Financial support and sponsorship

Partly supported by "Young Research Faculty Grant" provided by Sri Ramachandra University, India.

Conflicts of interest

There are no conflicts of interest.

REFERENCES

- Zinelis S, Eliades T, Eliades G. A metallurgical characterization of ten endodontic Ni-Ti instruments: Assessing the clinical relevance of shape memory and superelastic properties of Ni-Ti endodontic instruments. *Int Endod J* 2010;43:125-34.
- Parashos P, Messer HH. Rotary NiTi instrument fracture and its consequences. *J Endod* 2006;32:1031-43.
- Zhou HM, Shen Y, Zheng W, Li L, Zheng YF, Haapasalo M. Mechanical properties of controlled memory and superelastic nickel-titanium wires used in the manufacture of rotary endodontic instruments. *J Endod* 2012;38:1535-40.
- Shen Y, Zhou HM, Zheng YF, Peng B, Haapasalo M. Current challenges and concepts of the thermomechanical treatment of nickel-titanium instruments. *J Endod* 2013;39:163-72.
- Shen Y, Zhou HM, Zheng YF, Campbell L, Peng B, Haapasalo M. Metallurgical characterization of controlled memory wire nickel-titanium rotary instruments. *J Endod* 2011;37:1566-71.
- Gao Y, Gutmann JL, Wilkinson K, Maxwell R, Ammon D. Evaluation of the impact of raw materials on the fatigue and mechanical properties of ProFile Vortex rotary instruments. *J Endod* 2012;38:398-401.
- Thompson SA. An overview of nickel-titanium alloys used in dentistry. *Int Endod J* 2000;33:297-310.
- Alapati SB, Brantley WA, Iijima M, Clark WA, Kovarik L, Buie C, *et al.* Metallurgical characterization of a new nickel-titanium wire for rotary endodontic instruments. *J Endod* 2009;35:1589-93.
- ColteneEndo. HyflexCM Brochure. Available from: http://www.coltene.com/download.php?file_id=5085. [Last accessed on 2015 Mar 12].
- Testarelli L, Plotino G, Al-Sudani D, Vincenzi V, Giansiracusa A, Grande NM, *et al.* Bending properties of a new nickel-titanium alloy with a lower percent by weight of nickel. *J Endod* 2011;37:1293-5.
- Zhou H, Peng B, Zheng YF. An overview of the mechanical properties of nickel-titanium endodontic instruments. *Endod Topics* 2013;29:42-54.
- Peters OA, Gluskin AK, Weiss RA, Han JT. An *in vitro* assessment of the physical properties of novel Hyflex nickel-titanium rotary instruments. *Int Endod J* 2012;45:1027-34.
- Haapasalo M, Shen Y. Evolution of nickel-titanium instruments: From past to future. *Endod Topics* 2013;29:3-17.
- Lal DM, Renganarayanan S, Kalanidhi A. Cryogenic treatment to augment wear resistance of tool and die steels. *Cryogenics* 2001;41:149-55.
- Bensely A, Senthilkumar D, Lal DM, Nagarajan G, Rajadurai A. Effect of cryogenic treatment on tensile behavior of case carburized steel-815M17. *Mater Charact* 2007;58:485-91.
- Reasbeck RB. Improved tool life by the cryotough treatment. *Metallurgia* 1989;56:178-9.
- Singh PJ, Guha B, Achar DR. Fatigue life improvement of AISI 304L cruciform welded joints by cryogenic treatment. *Eng Fail Anal* 2003;10:1-12.
- Barron RF. Cryogenic treatment of metals to improve wear resistance. *Cryogenics* 1982;22:409-13.
- Vinothkumar TS, Miglani R, Lakshminarayanan L. Influence of deep dry cryogenic treatment on cutting efficiency and wear resistance of nickel-titanium rotary endodontic instruments. *J Endod* 2007;33:1355-8.
- Kim JW, Griggs JA, Regan JD, Ellis RA, Cai Z. Effect of cryogenic treatment on nickel-titanium endodontic instruments. *Int Endod J* 2005;38:364-71.
- Leskovsek V, Kalin M, Vizintin J. Influence of deep-cryogenic treatment on wear resistance of vacuum heat-treated HSS. *Vacuum* 2006;80:507-18.
- ASTM F2063-05. Specification for Wrought Nickel-titanium Shape Memory Alloys for Medical Devices and Surgical Implants. West Conshohocken, PA: ASTM International; 2005. Available from: <http://www.astm.org>. [Last accessed on 2015 May 14].
- ASTM G133-02. Standard Test Method for Linearly Reciprocating Ball-on-flat Sliding Wear. West Conshohocken, PA: ASTM International; 2002. Available from: <http://www.astm.org>. [Last accessed on 2015 May 14].
- Vimal AJ, Bensely A, Lal DM, Srinivasan K. Deep cryogenic treatment improves wear resistance of En 31 steel. *Mater Manuf Process* 2008;23:369-76.
- Darwin JD, Lal DM, Nagarajan G. Optimization of cryogenic treatment to maximize the wear resistance of 18% Cr martensitic stainless steel by Taguchi method. *J Mater Process Technol* 2008;195:241-7.
- Molinari A, Pellizzari M, Gialanella S, Straffellini G, Stiasny KH. Effect of deep cryogenic treatment on the mechanical properties of tool steels. *J Mater Process Technol* 2001;118:350-5.
- Ninan E, Berzins DW. Torsion and bending properties of shape memory and superelastic nickel-titanium rotary instruments. *J Endod* 2013;39:101-4.
- Uchil J, Fernandes FM, Mahesh KK. X-ray diffraction study of the phase transformations in NiTi shape memory alloy. *Mater Charact* 2007;58:243-8.
- Shen Y, Coil JM, Zhou H, Zheng Y, Haapasalo M. HyFlex nickel-titanium rotary instruments after clinical use: Metallurgical properties. *Int Endod J* 2013;46:720-9.
- Zhao NQ, Man HC, Cui ZD, Yang XJ. Structure and wear properties of laser gas nitrided NiTi surface. *Surf Coat Technol* 2006;200:4879-84.
- Vinothkumar TS, Kandaswamy D, Prabhakaran G, Rajadurai A. Microstructure of cryogenically treated martensitic shape memory nickel-titanium alloy. *J Conserv Dent* 2015;18:292-6.
- Abedini M, Ghasemi HM, Nili Ahmadabadi M. Tribological behavior of NiTi alloy in martensitic and austenitic states. *Mater Des* 2009;30:4493-7.
- Brockhurst P, Hsu E. Hardness and strength of endodontic instruments made from NiTi alloy. *Aust Endod J* 1998;24:115-9.

Access this article online

Quick Response Code:



Website:
www.eurjdent.com