




Endoscopic ultrasound-guided renal biopsy: an alternative to transjugular renal biopsy in high-risk patients

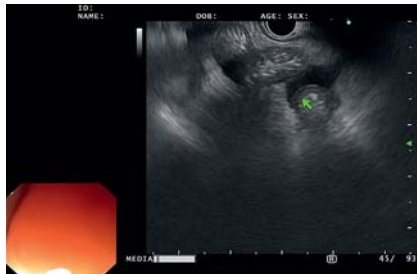

► **Fig. 1** Endoscopic ultrasonography showing interbowel fluid.

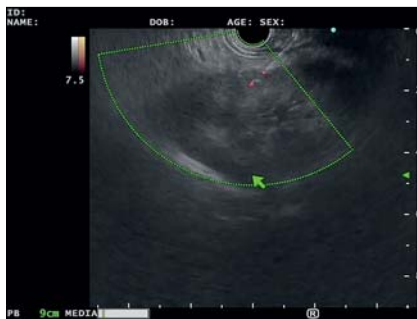

► **Fig. 2** Endoscopic ultrasound-guided fine-needle biopsy (FNB) taken from lower pole of left kidney.

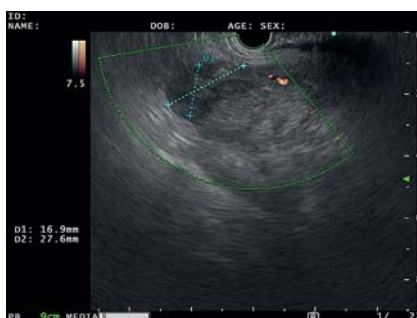

► **Fig. 3** Subcapsular hematoma in the lower pole of the left kidney, 27 × 17 mm in size.


A 32-year-old man with hepatocellular cancer who had undergone right hepatectomy 2 years previously presented with facial puffiness and abdominal distension. Ultrasound showed moderate ascites with normal kidneys. Serum albumin was 2.8 g/dL, hemoglobin 8.4 g/dL, platelet count 74 000/μL, and creatinine 1.7 mg/dL. Urine examination showed 3+ proteinuria and 3+ hematuria, while 24-hour urinary protein was 3030 mg/dL. Transjugular renal biopsy (TJRB) was advised after nephrology consultation, due to the ascites with thrombocytopenia, but the patient was not willing to undergo this procedure. Hence, endoscopic ultrasound (EUS)-guided biopsy with a linear echoendoscope (GIF UCT180; Olympus, Tokyo, Japan) was planned.

Examination revealed significant ascites with interbowel fluid (► **Fig. 1**). The left kidney was sampled via a transgastric approach, as the patient's surgically altered anatomy made scope positioning in the duodenal bulb precarious. A 22G Acquire needle (Boston Scientific, USA) was used to target the cortex of the lower pole of the left kidney, avoiding major medullary vessels. Two passes were made with three actuations each, with a slow-styleset pull-through (► **Fig. 2**; ► **Video 1**). A 2.7 × 1.6 cm subcapsular hematoma was seen (► **Fig. 3**). On visualization up to 10 minutes, no increase in the size of the hematoma could be seen. Ultrasound 12 hours after the procedure still revealed no increase in the hematoma. A 20-mm core was sent for histopathologic analysis and immunofluorescence studies (► **Fig. 4**). The diagnosis of focal segmental glomerulosclerosis was confirmed (► **Fig. 5**).

TJRB is the alternative to percutaneous biopsy in high-risk patients with ascites and thrombocytopenia [1]. EUS-guided fine-needle aspiration cytology of renal masses has been described in case series [2, 3], but sampling for primary diagnosis




► **Fig. 4** Core specimen (arrow) obtained with a 22G FNB needle.

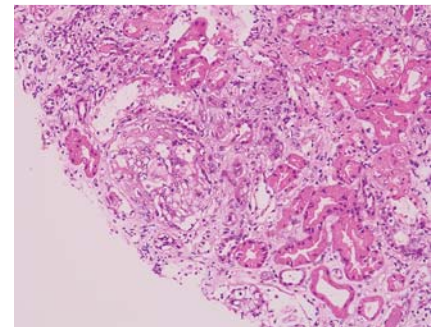

► **Fig. 5** Histopathologic analysis revealed a sclerosed glomerulus with mesangial widening with fibrosis in the interstitium, suggestive of focal segmental glomerulosclerosis.

of nephrotic syndrome has not been described. Unlike in EUS liver biopsy, where a 19G needle is used [4], in our case a 22G needle was used to reduce risk of bleeding. We were able to achieve an optimal sample for diagnosis using EUS, while avoiding radiation exposure and the use of contrast in a patient with compromised renal function.

Endoscopy_UCTN_Code_CCL_1AF_2AF_3AD

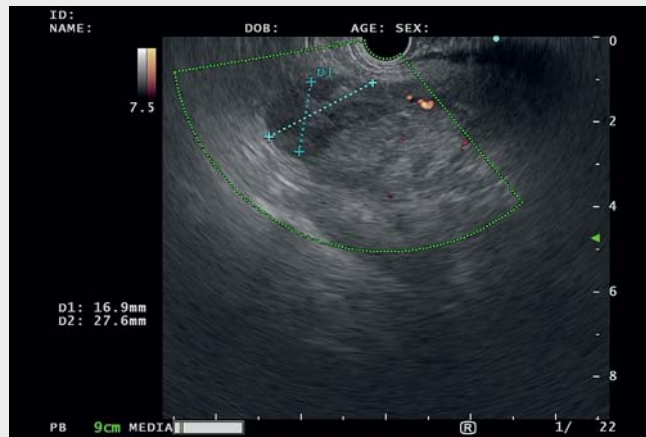

Video 1 Endoscopic ultrasound-guided kidney biopsy from the lower pole of the left kidney for evaluation of nephrotic syndrome.

the diagnosis of kidney lesions: a review. *World J Gastrointest Endosc* 2015; 7: 253–257

- [3] Law R, Wobker S, Grimm IS et al. Endoscopic ultrasonography-guided fine needle aspiration of kidney masses. *Gastroenterology* 2015; 148: 1282–1283
- [4] Patel HK, Saxena R, Rush N et al. A comparative study of 22G versus 19G needles for EUS-guided biopsies for parenchymal liver disease: are thinner needles better? *Dig Dis Sci* 2021; 66: 238–246

Bibliography

Endoscopy 2022; 54: E285–E286

DOI 10.1055/a-1519-6365

ISSN 0013-726X

published online 2.7.2021

© 2021. Thieme. All rights reserved.

Georg Thieme Verlag KG, Rüdigerstraße 14, 70469 Stuttgart, Germany

ENDOSCOPY E-VIDEOS

<https://eref.thieme.de/e-videos>



Endoscopy E-Videos is an open access online section, reporting on interesting cases

and new techniques in gastroenterological endoscopy. All papers include a high quality video and all contributions are freely accessible online. Processing charges apply (currently EUR 375), discounts and waivers acc. to HINARI are available.

This section has its own submission website at

<https://mc.manuscriptcentral.com/e-videos>

Competing interests

The authors declare that they have no conflict of interest.

The authors

Sridhar Sundaram¹, Prachi Patil¹, Aadish Jain¹, Utkarsh Chhanchure¹, Suman Kumar Ankathi¹, Shaila Khubchandani², Shaesta Mehta¹

- 1 Department of Digestive Diseases and Clinical Nutrition, Tata Memorial Hospital, Mumbai, India
- 2 Department of Pathology, Jaslok Hospital, Mumbai, India

Corresponding author

Sridhar Sundaram, MD, DM

Department of Digestive Diseases and Clinical Nutrition, Tata Memorial Hospital, Dr. E. Borges Road, Parel, Mumbai, Maharashtra 400012, India
drsridharsundaram@gmail.com

References

- [1] Rathod KR, Popat BA, Pandey A et al. Safety and effectiveness of transjugular renal biopsy: a single center study. *Indian J Nephrol* 2017; 27: 118–123
- [2] Lopes RI, Moura RN, Artifon E. Endoscopic ultrasound-guided fine-needle aspiration for