

Diameter of surgical versus endoscopic ultrasound-guided gastrojejunostomy: that much wider after all is said and done?


Whereas retrospective literature confirms the comparable clinical success of endoscopic ultrasound-guided gastrojejunostomy (EUS-GJ) and surgical gastrojejunostomy (SGJ) [1,2], no head-to-head comparison exists of their caliber and long-term patency.

We present one case of a patient receiving both procedures, offering an unusual opportunity for direct comparison (► **Video 1**).


A 52-year-old patient was diagnosed with gastric outlet obstruction owing to a duodenal B-cell lymphoma. EUS-GJ was performed using a 20-mm lumen-apposing metal stent (LAMS), followed by 18-mm balloon dilation [3] (► **Fig. 1**). Upon disease remission with chemotherapy, a blind-ended bulb resulted from scarring of the stenotic duodenal tract. Although the EUS-GJ was wide and patent (► **Fig. 2**), erosions were appearing on the jejunal side after 8 months (► **Fig. 2c**) and an SGJ was proposed owing to the uncertainty of long-term patency of the EUS-GJ and a potentially wider caliber of the SGJ. Following surgery, gastrointestinal follow-through (► **Fig. 3**) showed adequate flow through both anastomoses, but EUS-GJ seemed reduced in diameter 13 months after placement. LAMS extraction was planned, revealing significant granulation tissue overgrowth surrounding a stabilized fistula reduced in caliber (► **Fig. 3**).

On that occasion, the SGJ caliber was evaluated. Although the surgeon created an almost 5-cm incision, a 20-mm balloon perfectly fitted the final SGJ (► **Fig. 4**). Indeed, SGJ requires a linear incision of stomach and jejunal walls and latero-lateral suturing of their inferior and superior margins [4]. This elliptic anastomosis will become round after maturation and scarring, with a smaller final circular diameter compared to the initial linear cut (► **Fig. 5**).

Pending randomized data, this case suggests a comparable caliber of SGJ and

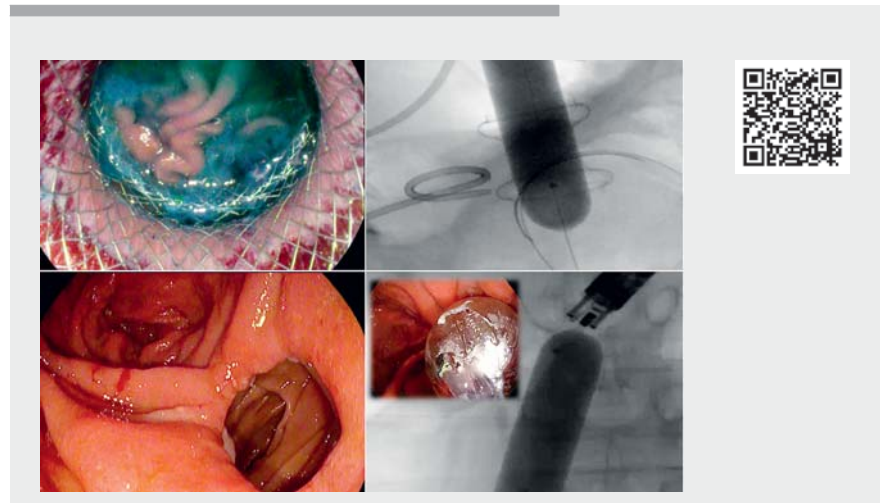

► **Video 1** A patient receiving both an endoscopic ultrasound-guided and a surgical gastrojejunostomy offered an unusual opportunity to compare the diameter of the 2 anastomoses.

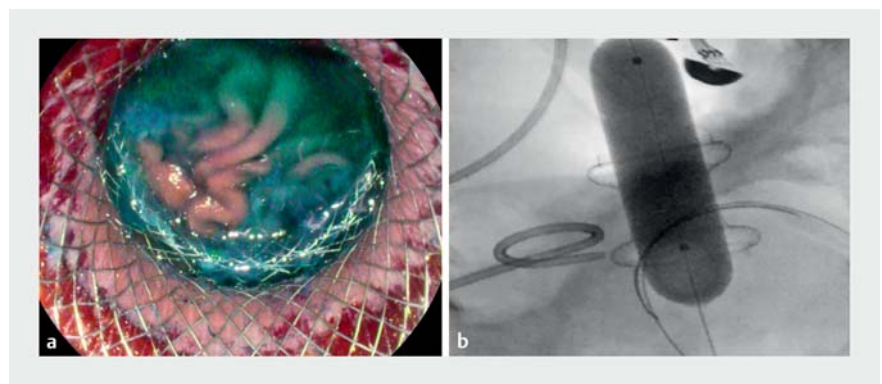


► **Fig. 1** Endoscopic ultrasound (EUS)-guided gastrojejunostomy after lumen-apposing metal stent (LAMS) placement. **a** Endoscopic view of the small intestine through the LAMS, with some blue fluid used for jejunal distention coming into the stomach. **b** Radiograph of 18-mm balloon dilating the 20-mm LAMS after placement.

EUS-GJ for a substantial part of their history, and therefore an assumed larger diameter should not be used as a reason to prefer SGJ. However, it also suggests that long-term LAMS friction may induce inflammatory responses deserving further elucidation, especially when advocating EUS-GJ use in benign disease.


Endoscopy_UCTN_Code_TTT_1AT_2AD

Competing interests

Michiel Bronswijk has consultancy agreements with Prion Medical – Taewoong. Schalk Van der Merwe holds the Cook and Boston-Scientific chair in interventional endoscopy and holds consultancy agreements with Cook, Pentax and Olympus. The remaining authors declare no COI relevant for this article.

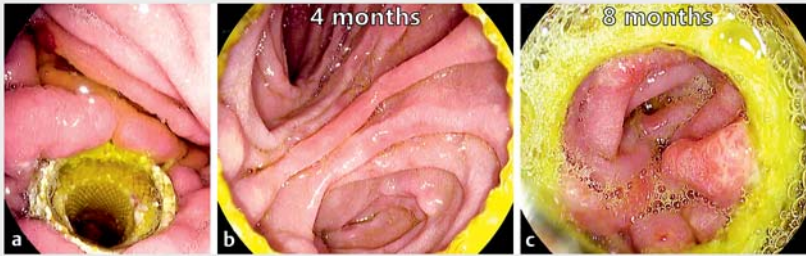

► **Fig. 2** Endoscopic follow-up of the endoscopic ultrasound-guided gastrojejunostomy (EUS-GJ). **a, b** Follow-up at 4 months: wide and patent EUS-GJ, with normotrophic mucosa on the jejunal side. **c** Follow-up at 8 months: initial erosions were seen on the jejunal side of the anastomosis.

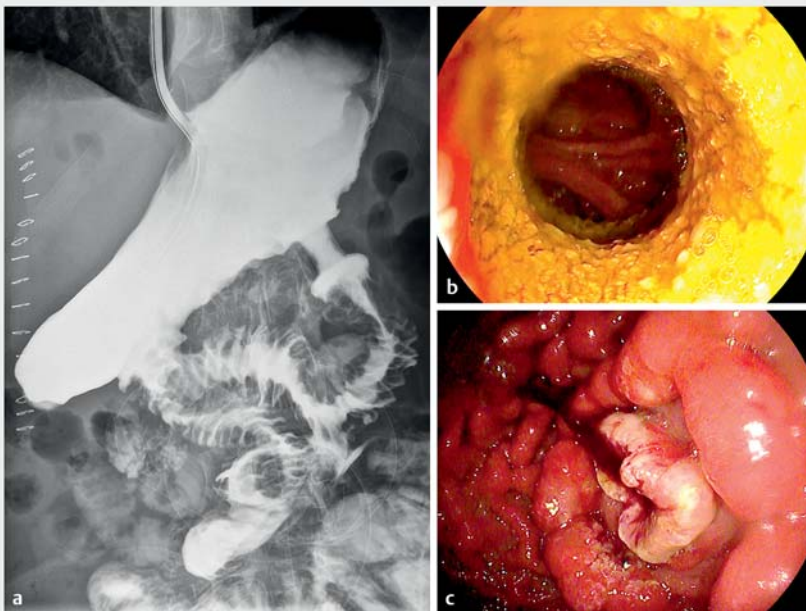

► **Fig. 3 a** Endoscopic follow-through showing adequate contrast flow through both anastomoses, although EUS-GJ diameter seemed slightly reduced after 13 months. **b, c** Endoscopy performed for lumen-apposing metal stent (LAMS) extraction 13 months after placement. **b** Endoscopic view of the LAMS reduced in caliber, not passable with a standard gastroscope. **c** After LAMS removal, significant granulation tissue overgrowth was visible surrounding a stabilized fistula reduced in caliber.

The authors

Giuseppe Vanella¹, Domenico Tamburrino²,
Francesco Vito Mandarino¹, Michiel
Bronswijk^{3,4}, Schalk Van der Merwe³,
Massimo Falconi², Paolo Giorgio Arcidiacono¹

- 1 Pancreatobiliary Endoscopy and Endosonography Division, Pancreas Translational & Clinical Research Center, IRCCS San Raffaele Scientific Institute, Milan, Italy
- 2 Pancreatic Surgery Unit, Pancreas Translational & Clinical Research Center, IRCCS San Raffaele Scientific Institute, Milan, Italy
- 3 Department of Gastroenterology and Hepatology, University Hospitals Gasthuisberg, University of Leuven, Leuven, Belgium.
- 4 Department of Gastroenterology and Hepatology, Imelda General Hospital, Bonheiden, Belgium


Corresponding author

Giuseppe Vanella, MD


Pancreatobiliary Endoscopy and Endosonography Division, Pancreas Translational & Clinical Research Center, IRCCS San Raffaele Scientific Institute, Vita-Salute San Raffaele University, Via Olgettina 60, 20132, Milan, Italy
Fax: +39-0226435609
vanella.giuseppe@hsr.it

References

- [1] Fan W, Tan S, Wang J et al. Clinical outcomes of endoscopic ultrasound-guided gastroenterostomy for gastric outlet obstruction: a systematic review and meta-analysis. *Minim Invasive Ther Allied Technol* 2020; 1–9. doi:10.1080/13645706.2020.1792500
- [2] Bronswijk M, Vanella G, van Malenstein H et al. Laparoscopic versus EUS-guided gastroenterostomy for gastric outlet obstruction: an international multicenter propensity score-matched comparison (with video). *Gastrointest Endosc* 2021. doi:10.1016/j.gie.2021.04.006

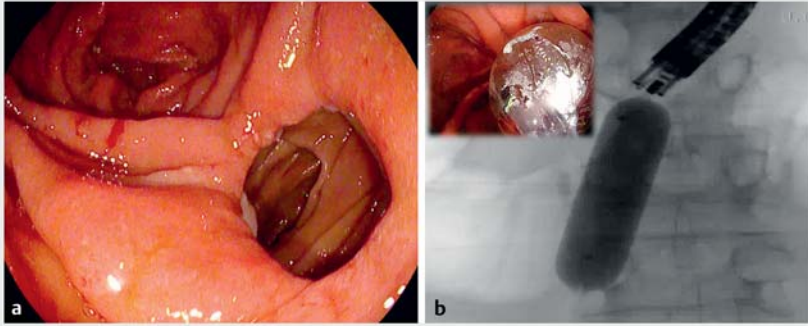

► **Fig. 4** Surgical gastrojejunostomy caliber evaluated with a 20-mm dilation balloon, perfectly fitting the anastomosis.

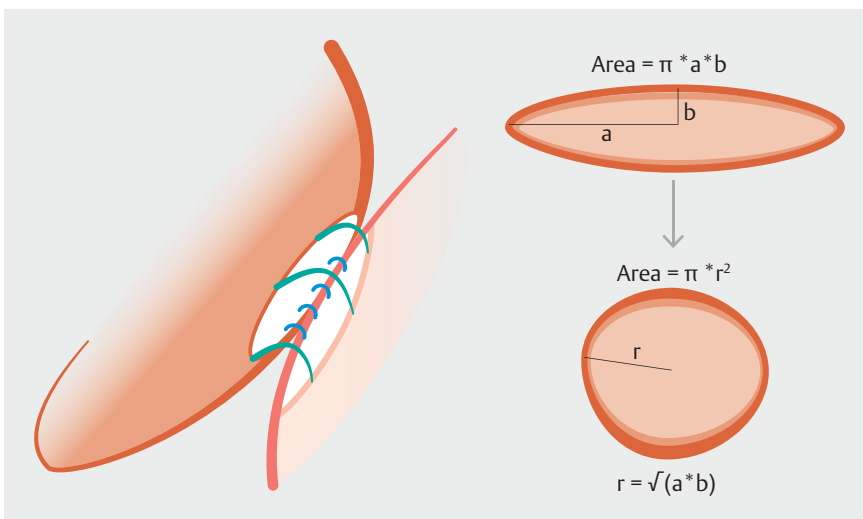

► **Fig. 5** Pictorial representation of a surgical gastrojejunostomy. Left) Procedure requires the approximation of stomach and jejunal loops, a linear incision of their walls, and a latero-lateral suturing of their inferior and superior margins. This creates an elliptic anastomosis, which turns round after maturation and scarring. As surface areas must remain unchanged, the diameter of the final circular anastomosis will be inferior to the surgically made linear cut. Because the area of an ellipse is $\pi * a * b$ (the 2 semi-axes of the ellipse) and the area of a circle is $\pi * r^2$ and the area cannot change during maturation, final radius of the circular anastomosis might be approximated to the square root of half the surgical linear incision.

- [3] Rossi G, Petrone MC, Vanella G et al. EUS-guided gastroenterostomy in a COVID-19-infected patient with duodenal stenosing lymphoma (with videos). *Endosc Ultrasound* 2021; 10: 221–223. doi:10.4103/EUS-D-20-00255
- [4] Rodríguez JI, Kutscher M, Lemus M et al. Palliative gastrojejunostomy in unresectable cancer and gastric outlet obstruction: a retrospective cohort study. *Ann R Coll Surg Engl* 2021; 103: 197–202. doi:10.1308/RCSANN.2020.7016

Bibliography

Endoscopy 2022; 54: E449–E451
 DOI 10.1055/a-1562-1274
 ISSN 0013-726X
 published online 17.9.2021
 © 2021. Thieme. All rights reserved.
 Georg Thieme Verlag KG, Rüdigerstraße 14,
 70469 Stuttgart, Germany

ENDOSCOPY E-VIDEOS

<https://ref.thieme.de/e-videos>



Endoscopy E-Videos is an open access online section, reporting on interesting cases and new techniques in gastroenterological endoscopy. All papers include a high quality video and all contributions are freely accessible online. Processing charges apply (currently EUR 375), discounts and waivers acc. to HINARI are available.

This section has its own submission website at
<https://mc.manuscriptcentral.com/e-videos>