

# Controlled Prospective Study on the Use of Systematic Simulator-Based Training with a Virtual, Moving Fetus for Learning Second-Trimester Scan: FESIM III

## Kontrollierte, prospektive Studie zur Erlernbarkeit von erweiterten Zweittrimesterschalls mittels simulationsbasiertem Ultraschalltrainings mit einem virtuellen, sich bewegenden Fetus: FESIM III

OPEN  
ACCESS



### Authors

Paula Freundt<sup>1†</sup>, Nasenien Nourkami-Tutdibi<sup>1†</sup>, Erol Tutdibi<sup>1</sup>, Paul Janzing<sup>1</sup>, Thomas von Ostrowski<sup>2</sup>, Martin Langer<sup>3</sup>, Michael Zemlin<sup>1</sup>, Johannes Steinhard<sup>4,5</sup>

### Affiliations

- 1 Hospital for General Pediatrics and Neonatology, Saarland University Medical Center, Homburg, Germany
- 2 Prenatal Medicine Dorsten, Dorsten, Germany
- 3 Practice for Gynecology and Women Health, LARA, Bocholt, Germany
- 4 Fetal Cardiology, Heart and Diabetes Center NRW, Ruhr University Bochum, Bad Oeynhausen, Germany
- 5 Prenatal Medical Center Münster, Münster, Germany

### Key words

prenatal detection rate, simulation-based medical education, fetal ultrasound, ultrasound simulation, second-trimester screening

received 13.10.2022

accepted after revision 16.11.2022

published online 07.03.2023

### Bibliography

Ultraschall in Med 2023; 44: e199–e205

DOI 10.1055/a-1984-8320

ISSN 0172-4614

© 2023. The Author(s).

This is an open access article published by Thieme under the terms of the Creative Commons Attribution-NonDerivative-NonCommercial-License, permitting copying and reproduction so long as the original work is given appropriate credit. Contents may not be used for commercial purposes, or adapted, remixed, transformed or built upon. (<https://creativecommons.org/licenses/by-nc-nd/4.0/>).

Georg Thieme Verlag KG, Rüdigerstraße 14,  
70469 Stuttgart, Germany

### Correspondence

Dr.med. Nasenien Nourkami-Tutdibi  
Hospital for General Pediatrics and Neonatology  
Saarland University Medical Center, Building 9, 66421  
Homburg, Germany  
[nasenien.nourkami@uks.eu](mailto:nasenien.nourkami@uks.eu)

### ABSTRACT

**Objectives** To analyze the feasibility of structured ultrasound simulation training (SIM-UT) in teaching second-trimester ultrasound screening using a high-end simulator with a randomly moving fetus.

**Methods** This was a prospective, controlled trial. A trial group of 11 medical students with minimal obstetric ultrasound experience underwent 12 hours of structured SIM-UT in individual hands-on sessions within 6 weeks. Learning progress was assessed with standardized tests. Performance after 2, 4, and 6 weeks of SIM-UT was compared with two reference groups ((A) Ob/Gyn residents and consultants, and (B) highly skilled DEGUM experts). Participants were asked to acquire 23 2nd trimester planes according to ISUOG guidelines in a realistic simulation B-mode with a randomly moving fetus as quickly as possible within a 30-minute time frame. All tests were analyzed regarding the rate of appropriately obtained images and the total time to completion (TTC).

**Results** During the study, novices were able to improve their ultrasound skills significantly, reaching the physician level of the reference group (A) after 8 hours of training. After 12 hours of SIM-UT, the trial group performed significantly faster than the physician group (TTC:  $621 \pm 189$  vs.  $1036 \pm 389$  sec.,  $p = 0.011$ ). Novices obtained 20 out of 23 2nd trimester standard planes without a significant time difference when compared to experts. TTC of the DEGUM reference group remained significantly faster ( $p < 0.001$ ) though.

**Conclusion** SIM-UT on a simulator with a virtual, randomly moving fetus is highly effective. Novices can obtain standard plane acquisition skills close to expert level within 12 hours of self-training.

### ZUSAMMENFASSUNG

**Ziel** Die Untersuchung des strukturierten, simulationsbasierten Ultraschalltrainings (SIM-UT) an einem High-End-Simulator mit einem sich zufällig bewegenden Fetus für das Erlernen des erweiterten Zweit-Trimester-Screenings.

† These authors contributed equally.

**Methoden** In einer prospektiven, kontrollierten Studie trainierten 11 Medizinstudierende mit minimaler gynäkologischer Ultraschall Erfahrung über 6 Wochen insgesamt 12 h SIM-UT in 12 Einzelsitzungen. Der Lernfortschritt wurde in einem standardisierten Test am Simulator regelmäßig überprüft: 23 Standardebenen eines erweiterten Screening-Protokolls gemäß ISUOG-Standard sollten ohne Hilfestellungen so schnell wie möglich innerhalb von 30 min am Simulator dargestellt werden. Die Ergebnisse wurden anhand desselben standardisierten Tests mit (A) 10 Gynäkolog\*innen und (B) 10 DEGUM-Expert\*innen als Referenzgruppen verglichen. Alle Tests wurden hinsichtlich der Rate korrekt dargestellter Ebenen und der Gesamtzeit der Untersuchung (TTC) ausgewertet.

**Ergebnisse** Im Laufe der Studie verbesserte die Interventionsgruppe ihre Leistung signifikant und erreichte nach 8 h SIM-UT das Niveau der Referenzgruppe (A). Nach 12 h SIM-UT waren die Studierenden signifikant schneller als die Referenzgruppe (A) (TTC:  $621 \pm 189$  vs.  $1036 \pm 389$  Sek.,  $p = 0,011$ ). Im Aufsuchen von 20 der 23 Ebenen unterschied sich die Geschwindigkeit der Interventionsgruppe nicht mehr signifikant von der der Expert\*innen. Die TTC der DEGUM-Expert\*innen blieb jedoch signifikant schneller ( $p < 0,001$ ).

**Schlussfolgerungen** SIM-UT an einem Simulator mit einem virtuellen, sich zufällig bewegenden Fetus ist hoch effektiv. Ultraschallanfänger\*innen erreichen Ärzt\*innenstandard innerhalb von 8 h eigenständigen Trainings.

## Introduction


For prenatal diagnostics, ultrasound (US) is the gold standard to assess the development of the fetus, amniotic fluid, and fetomaternal blood flow [1]. Technical improvements via high-resolution US imaging and routine screening allow diagnosis of minor and complex malformations [2]. However, the quality of care leaves room for improvement [3, 4]. Despite advanced technology and regular scans, prenatal detection rates of fetal malformations still remain low [4, 5]. Health and development surveillance of pregnant women helps to decrease perinatal morbidity and mortality [6]. An essential part of quality assurance is structured training for US novices, as it is demanded by specialist societies [7, 8, 3, 9]. Obstetrical US examinations are conducted by obstetricians/gynecologists (Ob/Gyn) with teaching embedded in the clinical routine. The German Institute for Quality and Efficiency in Health Care (IQWiG) analyzed prenatal US screening in terms of the successful detection of fetal anomalies and concluded in 2008 that there is a positive association between higher qualification of the examiner and the successful detection of fetal anomalies [10]. In Germany, independent US practice is regulated by successful completion of a specialist exam and the mandatory acquisition of a certain number of scans. For prenatal US certification, 300 utero-placental-fetal scans are required [11] without quality control. Neither medical students nor residents receive US training as part of their routine medical education. Residents are often lost with respect to how and when to receive US education and experience when facing an increasing workload [12, 3]. Ob/Gyn residents are confronted with a discrepancy between their perceived level of confidence in US examination and expectations placed on them during their clinical work [13]. Standardization of US curricula is demanded by educational committees, as well as medical students and physicians in training [7, 12, 3]. An approach to meet the challenges of US education and quality assurance is to train novices in simulated settings until a certain level of proficiency is achieved to begin clinical training [14]. Simulation-based ultrasound training (SIM-UT) is an effective teaching tool for Ob/Gyn US skills [8]. SIM-UT can increase trainees' accuracy with respect to locating standard planes, organ measurements, and ex-

amination speed [15, 16]. Trainees who underwent SIM-UT have significantly improved their clinical performance and patient-perceived quality of care [9, 17]. Simulation-based tests are as effective as live model-based evaluations for obstetrical US skill assessment [18, 19, 20]. Little is known about the effectiveness of SIM-UT for detailed 2<sup>nd</sup> trimester US examinations [15, 8] as the most important US scan in the detection of fetal anomalies [1, 21]. We aimed to analyze whether SIM-UT is applicable to train US novices in complex 2<sup>nd</sup> trimester protocols. In addition, we aimed to assess the training time and intensity needed for US novices to gain a certain level of professionalism. Finally, we wanted to analyze the learning success of novices after 6 weeks of SIM-UT in comparison to physicians and US experts.

## Materials and methods

### Study design and participants

The fetal simulation study III (FESIM III) was a prospective trial to assess the learning progress of ultrasound novices in 2<sup>nd</sup> trimester scans in comparison to two reference groups. 11 medical students from year 2 to 6 were included as novices. The inclusion criteria were a) enrollment as a student b) completion of the subject of anatomy, c) less than 10 hours of experience in gynecological or obstetrical US. Additionally, as reference groups, 10 Ob/Gyn physicians and 10 fetal US experts were included separately (► Fig. 1). A parallel trial (FESIM II) analyzed learning curves during SIM-UT for fetal echocardiography. All medical students attended an introductory 90-minute seminar, followed by individual training sessions with the US Mentor. Two training sessions were supervised by student tutors giving a 30-minute introduction to each participant. The following training sessions were completed by the participants alone. Student tutors were available for questions. The novices completed a one-hour session twice a week for a total of 12 hours of self-training per person during the training period. The training focused on the correct acquisition of standard planes as an essential basis for any sonographic assessment. Trainees were able to learn the standard planes in pathologic cases during individual SIM-UT. All tests were carried out on a

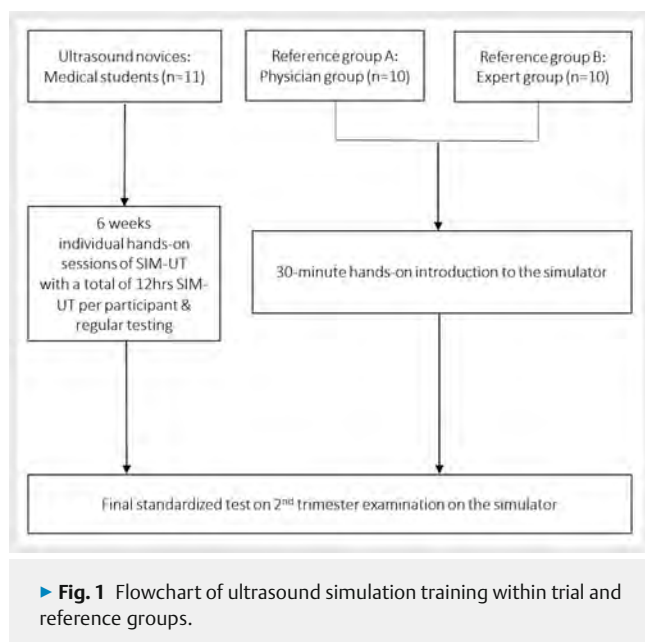

healthy, virtual fetus and the progress was analyzed in standardized tests every two weeks. Participants were asked to obtain and freeze all 23 correct standard views as quickly as possible with a moving fetus. Tests were carried out under real life examination conditions with all aids of the simulator being removed. The points in time when participants froze or unfroze an image or decided to abort the search within a certain standard plane were recorded. In examination mode, the US simulator automatically rated the obtained standard view as correct or incorrect after the completion of the examination. During the trial we noticed that the simulator sometimes rated correct planes as incorrect. Therefore, a second level of examination had to be implemented. If a captured plane was rated as incorrect by the simulator, a scientific expert panel consisting of three fetal US experts was considered to rate the obtained views either as correct or incorrect independently by retrospective video rating. The expert panel was comprised of members of the quality securing committee ("KVWL-Qualitätssicherungskommission") certified at least level II according to the "Deutsche Gesellschaft für Ultraschall in der Medizin" (DEGUM – German society for ultrasound in medicine). Planes were reevaluated using the grades used in the German school system, ranging from "1 – very good" to "6 – insufficient". The average grade of the three standard planes was calculated. Standard planes with average grades "1–4" were retrospectively re-evaluated as correctly obtained.

## Ultrasound Simulator

Our study was conducted on the Simbionix US Mentor ultrasound simulator (Simbionix, Beit Golan, Israel) consisting of a mannequin, various sham US probes, a touchscreen with a built-in PC, footswitch, and the "electronic box" as the central computing device connected to the transmitter. The latter, a hand-sized box attached to the back of the mannequin, emits a magnetic field, which is detected by built-in sensors of the sham US probes. This enables the simulator to locate the exact position of the probe

and the simulator renders a real-time image of a simulated fetus. This image calculation relies on a virtual fetus, that was generated using MRI volume data. The utilization of a virtual fetus enables the US Mentor to simulate fetal movements while scanning to create a realistic examination environment. This feature is unique to the US Mentor. The virtual fetus also facilitates the simulation of various artifacts and enables the implementation of malformations. The 2<sup>nd</sup> trimester module consisted of six modules, comprised of anatomy practice, one module with a healthy randomly moving fetus, and four randomly moving fetuses with different malformations. 23 standard views were selected for the practice of a detailed 2<sup>nd</sup> trimester scan. The Ob/Gyn module is designed in compliance with ISUOG guidelines. All planes of the sonomorphological scan of the German Maternity Guidelines IIb, the standard screening for 2<sup>nd</sup> trimester US, were included [1] (► **Table 1**). All standard planes according to DEGUM level II necessary for a detailed scan were included in the trial except for special heart planes which were analyzed in a separate study (FESIM II) focusing on fetal echocardiography [22]. ► **Fig. 2** demonstrates the US Mentor and different training modes. The reference groups received a questionnaire to quantify previous US experience, information regarding their professional career, such as specialist degree or level of DEGUM qualification.

## Statistical Analysis


After completion of the examinations, the time intervals needed by the participants to obtain the correct standard views were calculated using Microsoft Excel. The rate of appropriate images (RAI) was defined as the percentage of correctly obtained standard planes out of all standard planes. Total time to completion (TTC) was defined as the timespan needed by participants to obtain all 23 standard planes. Statistical analysis was performed using IBM SPSS Statistics 27. Paired non-parametric tests (Friedman and Wilcoxon) were used to compare RAI and TTC of the trial group between their three examinations after 2, 4, and 6 weeks. With non-parametric unpaired tests (Kruskal-Wallis and Mann-Whitney U), we compared performance values between novices, physicians, and DEGUM experts. A value of  $p < 0.05$  was considered significant.

## Results

11 medical students from year 2 to 6 were compared using a standardized test with the two reference groups (A) and (B). The experience levels of the reference groups for Ob/Gyn US are indicated in ► **Table 2**. The trial group benefitted from significant learning progress during the entire training period. In terms of accuracy, the group reached a medium score of  $94.9 \pm 6.7\%$  correctly obtained images after two weeks of SIM-UT and improved it to  $98.0 \pm 3.6\%$  after four weeks of training. They were able to reach the physicians' RAI after 4 weeks, i. e., 8 hours of self-training ( $98.0 \pm 3.6\%$  vs.  $96.5 \pm 4.5\%$ ). All members of the DEGUM expert group continued to have a higher RAI of 100%, even though this difference was not statistically significant ( $p$  overall = 0.062). However, there was a significant difference in RAI between the students' first test and the expert group ( $p < 0.008$ ). The TTC needed

► **Table 1** Standard planes and corresponding organs according to DEGUM guidelines.

Region	Plane	Region	Plane
Fetal head	Midline facial profile (MFP)	Abdomen	Abdomen with stomach (Abd)
	Coronal face (CF)		Umbilical cord insertion (Umb)
	Orbits		Kidneys coronal (Kidcor)
Brain	Transventricular		Kidneys axial (Kidax)
	Transthalamic	Limbs	Bladder transverse
	Transcerebellar		Humerus
Spine	Neck sagittal		Radius + ulna (RadUL)
	Spine sagittal		Hand
Thorax	Four-chamber view (4CV)		Femur
	Diaphragm/left lung (LeftLung)		Tibia + fibula (TibFib)
	Diaphragm/right lung (RightLung)	Placenta	Foot
			Placenta

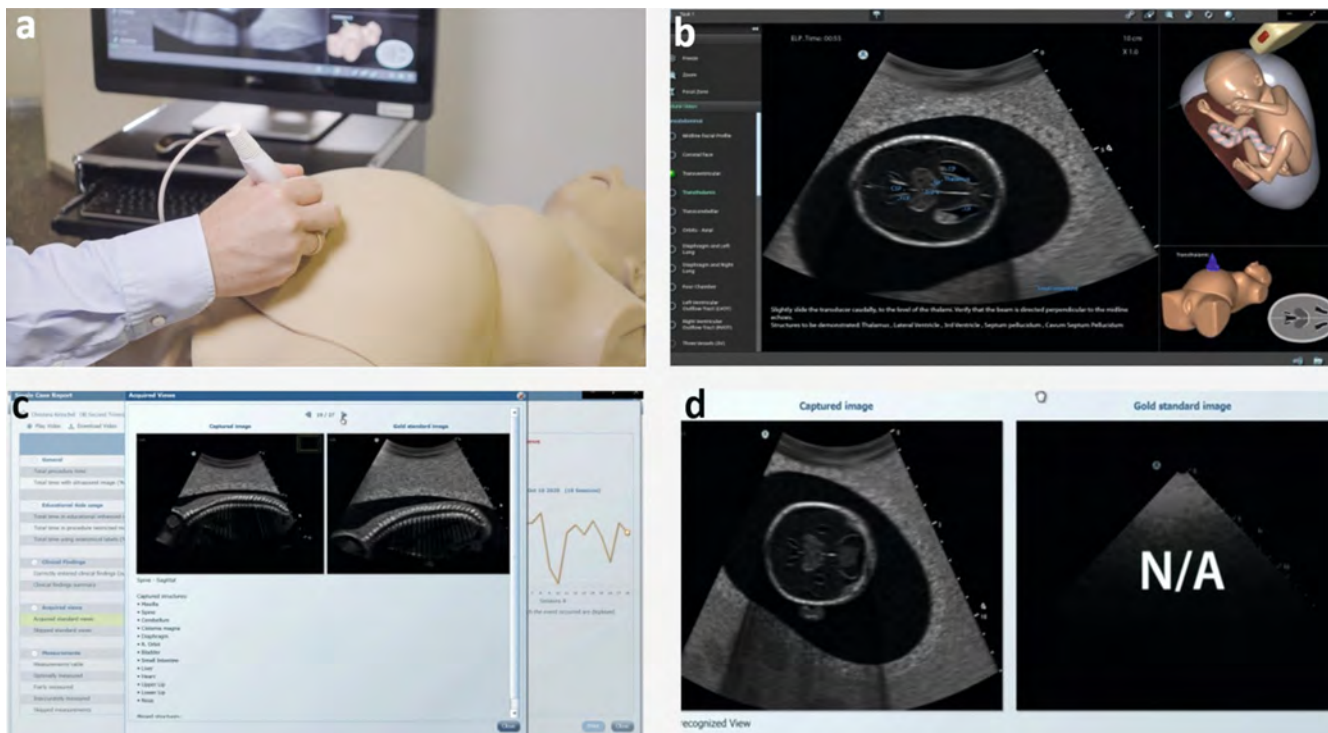► **Fig. 2** a–d US simulator equipment, (b) screen in learning mode: thalamic plane, (c) captured image with gold standard: spine, (d) captured plane rated as incorrect/not identified by simulator: cerebellar plane.


by the trial group to obtain all 23 standard planes shortened significantly over the training period (► **Fig. 3**). The score of  $1238 \pm 283$  seconds in the first test after two weeks of SIM-UT decreased to  $620 \pm 189$  seconds (average time per plane 27 seconds) after six weeks of training ( $p$  overall  $< 0.001$ ). After six weeks of self-training, the trial group scored a significantly faster TTC than the reference group of physicians ( $620 \pm 189$  vs.  $1036 \pm 389$  seconds,  $p < 0.001$ ) while the expert group remained significantly fas-

ter in its overall performance ( $443 \pm 243$  seconds,  $p < 0.001$ ). Similar results show the TTC of obtaining the planes for basic fetal biometry (transthalamic, abdominal, femur, and placental planes) (► **Fig. 4**). Regarding the time to obtain single standard planes, significant differences between the groups can be found in 8/23 planes. In 4 out of 8 planes, the trial group performed significantly faster than the physician group, while significant differences in time to obtain single standard planes showed no significant differ-




► **Table 2** Ultrasound experience of reference groups.

	Specialists	Residents	Median of Ob/Gyn US scans	Minimum number of scans performed	Maximum number of scans performed	Total number of scans performed
Reference group (A) Physician group, n = 10	2	8	750	130	40,000	48,130
Reference group (B) Expert group, n = 10	10	0	15,000	8,000	80,000	264,000

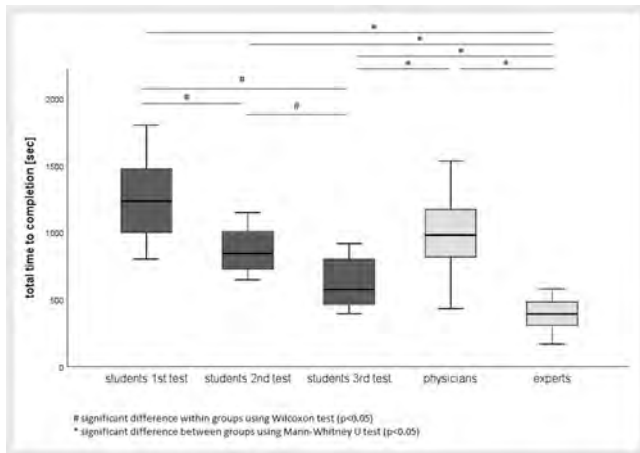

► **Fig. 3** Total time to completion of all 23 planes by study group.

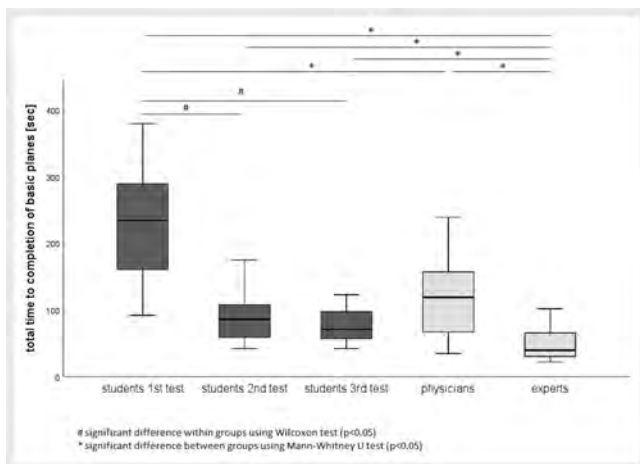


► **Fig. 4** Total time to completion of all basic planes by study group.

ence between novices and DEGUM experts for 20/23 2<sup>nd</sup> trimester standard planes after six weeks of SIM-UT (► **Fig. 5**). There was a significant difference for two planes of the basic fetal biometry planes, as DEGUM experts performed significantly faster than the reference (A) and trial groups. There was an overall of 268 obtained images that had to be reevaluated by the expert panel. Subsequently, 32 of the 268 images were evaluated as insufficient.

## Discussion

Advantages of SIM-UT include familiarization with US machines, acquisition of hand-eye coordination, anatomy standard planes, and examinations prior to clinical training on patients [23]. In our study we aimed to analyze these effects in learning curves for an extended detailed 2<sup>nd</sup> trimester examination protocol, since many fetal malformations present in planes beyond measuring fetal biometry [6, 5]. This is the first study to analyze training progress of US novices on a high-end simulator with a moving virtual fetus. Former studies on SIM-UT criticized the lack of fetal movement of US simulators [15]. The median experience of the physician group in our trial is about the same as the German standard for specialists in obstetrics, thus reflecting the skill level of basic US screening in Germany [11]. Their average group performance may be considered as representative for Ob/Gyn physicians in Germany since the group included physicians ranging from 1<sup>st</sup> year residency to consultant level. The fact that the trial group outperformed the physician group was unexpected and one major significant finding of our study. One reason might be insufficient supervision or a lack of structured US training associated with decreased US performance [23]. Some planes included in the protocol of the test were beyond basic screening and thus not necessarily applied in physicians' daily practice. Considering only standard planes, the trial group reached the physicians' skill level in the acquisition of basic standard planes but outperformed them significantly in the acquisition of the extended screening protocol. Therefore, residents, and even Ob/Gyn specialists in basic care will most likely benefit from SIM-UT in addition to their clinical training regardless of the number of performed scans upfront in their clinical routine. The strengths of the study include the highly qualified expert group consisting of only certified DEGUM experts with total experience of 264,000 US scans. Data from the standardized hands-on test, which was collected to analyze learning progress and to measure the performance of the three groups, discriminated between the different US competence levels of the groups. Subsequently, the expert group performed significantly better, while the physician group outperformed the trial group in terms of accuracy until the trial group gained experience of 8 hours of SIM-UT. That indicates the realism of the simulator, the possibility of assessing different US competence levels with a standardized hands-on simulator test, and the feasibility of learning 2<sup>nd</sup> trimester scans by structured SIM-UT even with no to minimum experience. Simulation-based examinations for the assessment have already been shown to be a useful method [18, 19,

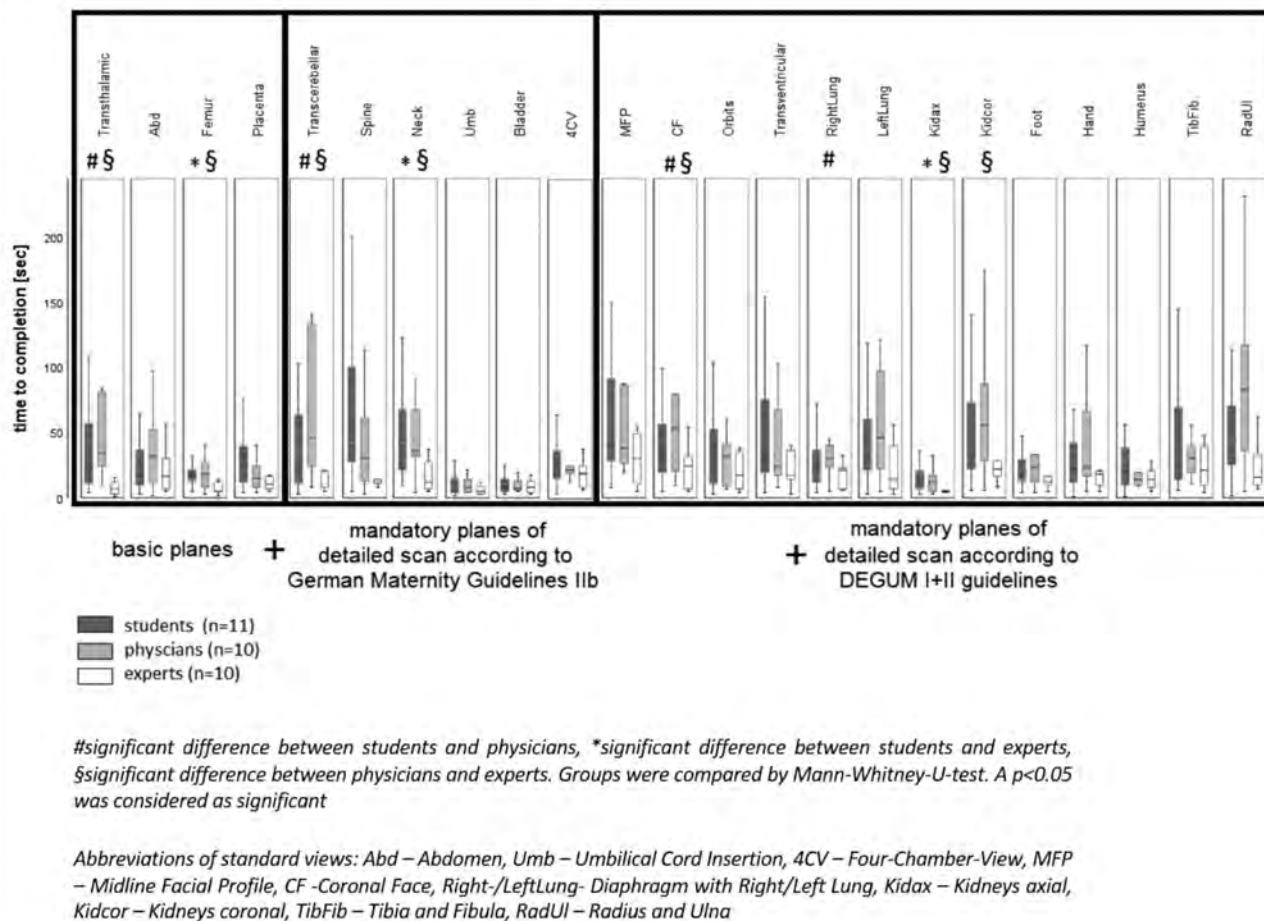

► **Fig. 5** Boxplot showing the distribution of total time to completion of single planes between trial group (students), reference group (A) (physicians), and reference group (B) (experts).

20]. If competence levels and skills can be assessed in a reliable way with US simulators, simulation-based tests could be an answer to long demanded accreditation and quality assurance for prenatal US [7]. Another strength of our study is the length of the intervention period, providing structured SIM-UT on a regular basis over six weeks, and the extent of the practiced examination protocol. Throughout the training period, the trial group recorded a significant decrease in TTC between each test. At the end of the training period, there were only three standard views that were accomplished significantly faster by the expert reference group. This crucial finding demonstrates that even very difficult standard views of extended protocols can be learned with SIM-UT. The positive feedback matches previous data about SIM-UT. SIM-UT is accepted among trainees in postgraduate training and is considered an essential part of their US education [24]. A limitation was the number of trial participants, which had to be kept limited, to allow enough time for training and skill progress testing. In detail, one simulator was available and shared with a parallel study with another group of 11 participants. Overall, 22 trainees each trained 2 hours per week on one simulator. Remaining time capacities were utilized to test skill progress and to evaluate the reference groups. As another limitation, we noticed a high rate of clinically

properly obtained images that were not assigned to the matching standard plane. 268 views did not meet the simulator's criteria whereas after expert panel review only 32/268 were classified as clinically insufficient. This discrepancy raises the question how the simulator evaluates the obtained images and when and in which situation the standard planes are rejected. In our experience, the tolerance should be adjusted for the acceptance of planes. Overall, simulators provide a safe learning space, with examinations being reproducible and cost-efficient [25]. In a standardized simulated setting trainees can focus on obtaining correct standard views to be able to detect fetal anomalies [26]. Individual different fetal and maternal physical characteristics can challenge sonographers and have not yet been implemented into the simulated examination conditions. Regardless of the latter, there is consensus regarding the efficacy and feasibility of SIM-UT in Ob/Gyn US [15, 16, 8, 9, 17]. The transferability of SIM-UT to real patients is part of successor trials. The quality of US examinations is significantly limited by the experience of the US operator, regardless of being a physician or technical sonographer [7]. Most importantly, while training US skills independent of mode of training (simulator vs. real patients), knowledge of US machines, technical pitfalls, and the knowledge behind image generation should be an

inevitable part of all US teaching [27]. Residents should have the opportunity to train on US simulators, as errors on real patients can effectively be limited through SIM-UT [28]. Structured SIM-UT is a highly effective tool to learn basic and extended prenatal US. While enabling significant skill acquisition within short periods, it provides a safe and learner-centered atmosphere and can be conducted independently during medical curricula and residency training programs. In an age of virtual technology, physicians should benefit from these realistic simulations of diagnostic and therapeutic procedures, in addition to their daily clinical practice [28]. Overall, standardized hands-on tests on US simulators are a reliable tool to assess operator skills and assure quality standards of US examinations.

## Conflict of Interest

The authors declare that they have no conflict of interest.

## References

- [1] Gemeinsamer Bundesausschuss. Richtlinien des Gemeinsamen Bundesausschusses über die ärztliche Betreuung während der Schwangerschaft und nach der Entbindung („Mutterschafts-Richtlinien“). In: Bundesanzeiger Nr. 60 a vom 27. März 1986; zuletzt geändert am 24. April 2014 veröffentlicht im Bundesanzeiger AT 27.06.2014 B3 in Kraft getreten am 28. Juni 2014. 2014 [cited 2021]. [https://www.g-ba.de/downloads/62-492-883/Mu-RL\\_2014-04-24.pdf](https://www.g-ba.de/downloads/62-492-883/Mu-RL_2014-04-24.pdf)
- [2] Eik-Nes SH. The 18-week fetal examination and detection of anomalies. *Prenat Diagn* John Wiley & Sons, Ltd 2010; 30: 624–630
- [3] Salvesen KA, Lees C, Tutschek B. Basic European ultrasound training in obstetrics and gynecology: Where are we and where do we go from here? *Ultrasound in Obstetrics and Gynecology*. John Wiley & Sons, Ltd 2010; 36: 525–529
- [4] Schwedler G, Lindinger A, Lange PE et al. Frequency and spectrum of congenital heart defects among live births in Germany: A study of the competence network for congenital heart defects. *Clin Res Cardiol* Springer 2011; 100: 1111–1117
- [5] Schmand C, Misselwitz B, Hudel H et al. Analysis of the Results of Sonographic Screening Examinations According to the Maternity Guidelines Before and After the Introduction of the Extended Basic Screening (IIB Screening) in Hesse. *Ultraschall der Medizin – Eur J Ultrasound* Georg Thieme Verlag KG 2022. doi:10.1055/a-1778-3585.
- [6] Kähler C, Schramm T, Bald R et al. Updated DEGUM quality requirements for the basic prenatal screening ultrasound examination (DEGUM Level I) between 18+0 and 21+6 weeks of gestation. *Ultraschall der Medizin* Georg Thieme Verlag 2020; 41: 499–503
- [7] Benacerraf BR, Minton KK, Benson CB et al. Proceedings: Beyond ultrasound first forum on improving the quality of ultrasound imaging in obstetrics and gynecology. *J Ultrasound Med* John Wiley and Sons Ltd 2018; 37: 7–18. doi:10.1002/jum.14504
- [8] Nayahangan LJ, Dietrich CF, Nielsen MB. Simulation-based training in ultrasound-where are we now? *Ultraschall in der Medizin*. Georg Thieme Verlag 2021; 42: 240–244
- [9] Taksøe-Vester C, Dyre L, Schroll J et al. Simulation-Based Ultrasound Training in Obstetrics and Gynecology: A Systematic Review and Meta-Analysis. *Ultraschall der Medizin – Eur J Ultrasound* 2021; 42: e42–e54. doi:10.1055/a-1300-1680
- [10] IQWiG (Institut für Qualität und Wirtschaftlichkeit im Gesundheitswesen). Ultraschallscreening in der Schwangerschaft: Testgüte hinsichtlich der Entdeckungsrate fetaler Anomalien 2008.
- [11] Kassenärztliche Bundesvereinigung. Qualitätssicherungsmaßnahmen nach § 135 Abs. 2 SGB V zur Ultraschalldiagnostik (Ultraschallvereinbarung) (Anlage 3 BMV-Ä). In: *Deutsches Ärzteblatt International*. 2021.
- [12] Recker F, Barth G, Lo H et al. Students' Perspectives on Curricular Ultrasound Education at German Medical Schools. *Front Med Frontiers Media S.A.*; 2021; 8: 758255
- [13] Tolsgaard MG, Rasmussen MB, Tappert C et al. Which factors are associated with trainees' confidence in performing obstetric and gynecological ultrasound examinations? *Ultrasound Obstet Gynecol* John Wiley and Sons Ltd 2014; 43: 444–451
- [14] Jensen JK, Dyre L, Jørgensen ME et al. Simulation-based point-of-care ultrasound training: a matter of competency rather than volume. *Acta Anaesthesiol Scand* Blackwell Munksgaard 2018; 62: 811–819
- [15] Burden C, Preshaw J, White P et al. Usability of virtual-reality simulation training in obstetric ultrasonography: A prospective cohort study. *Ultrasound Obstet Gynecol* John Wiley & Sons, Ltd 2013; 42: 213–217
- [16] Lous M Le, Tsatsaris V, Tesnière A et al. Improving students' ability to perform a standardized foetal biometry plane using ultrasound simulators. *J Gynecol Obstet Hum Reprod Elsevier Masson SAS* 2017; 46: 439–443. doi:10.1016/j.jogoh.2017.04.004
- [17] Tolsgaard MG, Ringsted C, Rosthøj S et al. The Effects of Simulation-based Transvaginal Ultrasound Training on Quality and Efficiency of Care. *Ann Surg Lippincott Williams and Wilkins* 2017; 265: 630–637. doi:10.1097/SLA.0000000000001656
- [18] Burden C, Preshaw J, White P et al. Validation of virtual reality simulation for obstetric ultrasonography: A prospective cross-sectional study. *Simul Healthc* 2012; 7: 269–273. doi:10.1097/SIH.0b013e3182611844
- [19] Chalouhi GE, Bernardi V, Gueneuc A et al. Evaluation of trainees' ability to perform obstetrical ultrasound using simulation: challenges and opportunities. *Am J Obstet Gynecol* Mosby Inc 2016; 214: 525.e1–525.e8
- [20] Madsen ME, Konge L, Nørgaard LN et al. Assessment of performance measures and learning curves for use of a virtual-reality ultrasound simulator in transvaginal ultrasound examination. *Ultrasound Obstet Gynecol* John Wiley and Sons Ltd 2014; 44: 693–699. doi:10.1002/uog.13400
- [21] Zollner U, Rehn M, Girschick G et al. Sonografische Auffälligkeiten des fetalen ZNS im Zweittrimesterscreening – Abklärung nach neuen Mutterschaftsrichtlinien. *Z Geburtshilfe Neonatol Z Geburtshilfe Neonatol* 2012; 216: 1–10
- [22] Merz E, Eichhorn KH, Kaisenberg C von et al. Aktualisierte Qualitätsanforderungen an die weiterführende differenzierte Ultraschalluntersuchung in der pränatalen Diagnostik (= DEGUM-Stufe II) im Zeitraum von 18 + 0 bis 21 + 6 Schwangerschaftswochen. *Ultraschall der Medizin – Eur J Ultrasound* 2012; 33: 593–596
- [23] Tolsgaard MG. Assessment and learning of ultrasound skills in obstetrics & gynecology. *Dan Med J* 2018; 65: 1–25
- [24] Patel H, Chandrasekaran D, Myriokefalitaki E et al. The Role of Ultrasound Simulation in Obstetrics and Gynecology Training. *Simul Healthc J Soc Simul Healthc Lippincott Williams and Wilkins* 2016; 11: 340–344. doi:10.1097/SIH.0000000000000176
- [25] Carolan-Rees G, Ray AF. The ScanTrainer obstetrics and gynaecology ultrasound virtual reality training simulator: A cost model to determine the cost viability of replacing clinical training with simulation training. *Ultrasound SAGE Publications Ltd* 2015; 23: 110–115
- [26] Nisselrooij AEL Van, Teunissen AKK, Clur SA et al. Why are congenital heart defects being missed? *Ultrasound Obs Gynecol* 2020; 55: 747–757
- [27] Pinto A, Pinto F, Faggian A et al. Sources of error in emergency ultrasonography 2013.
- [28] Ziv A, Root Wolpe P, Small SD et al. Simulation-based medical education: An ethical imperative. In: *Academic Medicine*. Hanley and Belfus Inc 2003; 78: 783–788