

Endoscopic submucosal dissection of an esophageal tumor using a transnasal endoscope without sedation

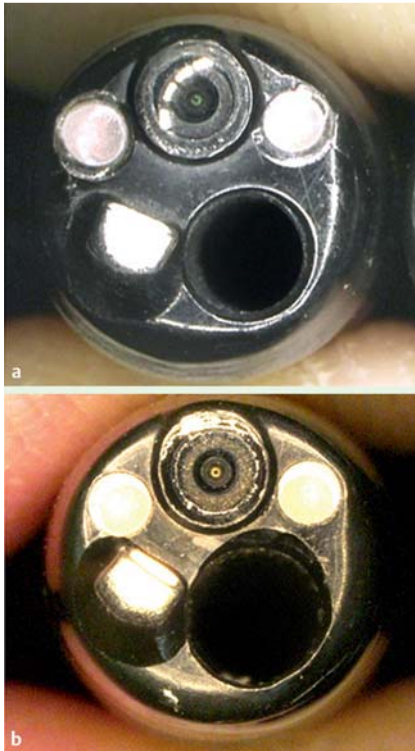


Fig. 1 Comparison of the EG-580NW2 with the EG-580NW transnasal endoscope. **a** EG-580NW has an instrument channel with 2.0mm inner diameter. **b** EG-580NW2 has an instrument channel with 2.4mm inner diameter.

Endoscopic submucosal dissection (ESD) within a narrow lumen is considered difficult. When ESD is conducted transorally for an esophageal tumor, the patient must be under sedation. We have already reported ESD using a transnasal endoscope in the pharynx without sedation [1]. Here, we report the first case of transnasal ESD for esophageal cancer without sedation.

The transnasal endoscope we used was the EG-580NW2 (Fujifilm, Tokyo, Japan), newly developed for the treatment of upper gastrointestinal lesions, which has an instrument channel with 2.4mm inner diameter although its distal end diameter is 5.8mm (Fig. 1). In addition, the EG-580NW2 can be used with a high-frequency electrosurgical system. We performed ESD for esophageal cancer using this endoscope with Nanoshooter, an original attachment hood [1]. The lesion appeared as a brownish area, and irregular vessels were recognized by using the narrow band imaging optical zoom (Fig. 2). The endoscope was inserted transnasally without sedation and a 1:1 mixture of glycerol and 0.4% hyaluronic acid [2] was injected into the submucosal layer (Fig. 3a). Once the lesion had been lifted, mucosal resection was performed at

the oral end of the lesion (Fig. 3b). Then, a J-turn was made in the gastric lumen, the scope was pulled up to the esophageal lumen, and the mucosa at the anal end of the lesion was fully resected (Fig. 3c). After completely resecting and trimming around the lesion, we used a snare to resect the lesion, to reduce procedure time (Fig. 4, Video 1). The total time taken was approximately 25 minutes. Our method shortened the time required to perform ESD in the esophagus because the anal end of the lesion was easily and completely resected using a J-turn. Moreover, the procedure was conducted without the risk associated with sedation and with little pain for the patient. The new EG-580NW2 transnasal endoscope is a very useful device for ESD.

Video 1

Procedure for transnasal endoscopic submucosal dissection of esophageal cancer.

Endoscopy_UCTN_Code_TTT_1AO_2AG

Competing interests: None

Masakatsu Nakamura¹, Hisakazu Shiroeda¹, Tomomitsu Tahara², Tomoyuki Shibata², Tomiyasu Arisawa¹

¹ Department of Gastroenterology, Kanazawa Medical University, Ishikawa, Japan

² Department of Gastroenterology, Fujita Health University, Aichi, Japan

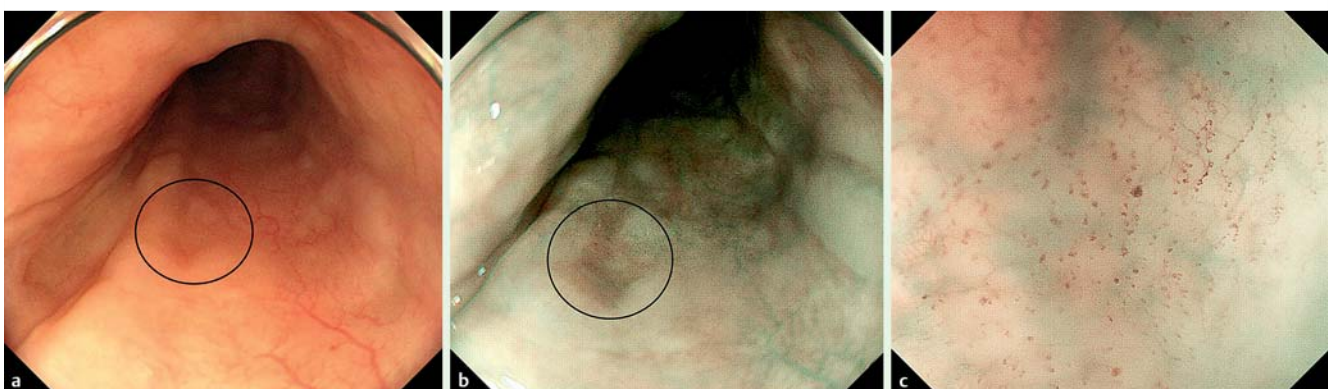


Fig. 2 The cancer in the esophagus. **a** Cancer lesion (encircled). **b** On narrow band imaging (NBI), the lesion appeared as a brownish area. **c** NBI optical zoom showed irregular vessels.

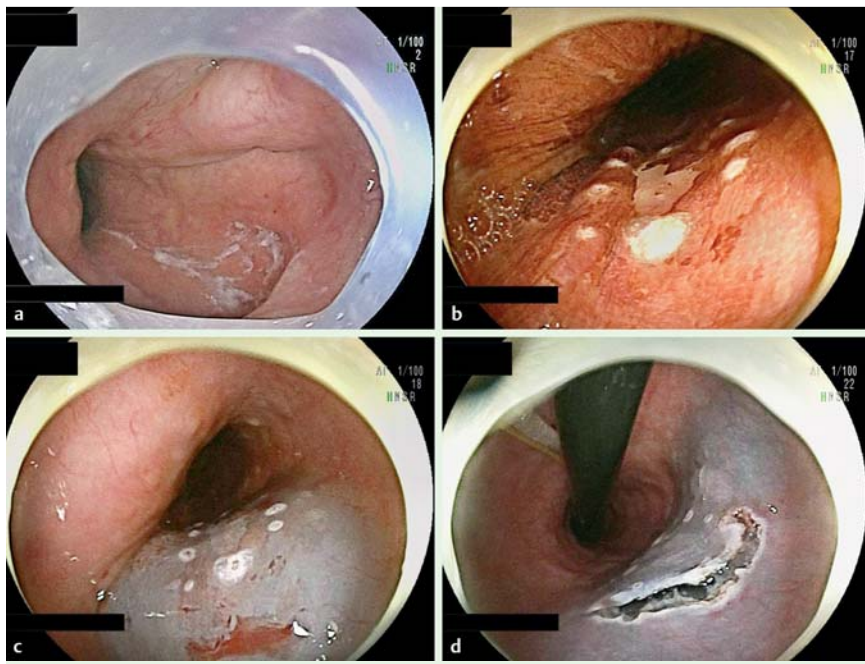


Fig. 3 Procedure for endoscopic submucosal dissection using a transnasal endoscope with Nano-shooter hood. **a** The endoscope with Nano-shooter attached was inserted transnasally. **b** The lesion was not stained with Lugol solution. A mixture of glycerol and hyaluronic acid was injected into submucosal layer, and the mucosal layer at the oral end of the lesion was incised. **c** Next, the mucosal layer at the anal end was incised, using a J-turn.

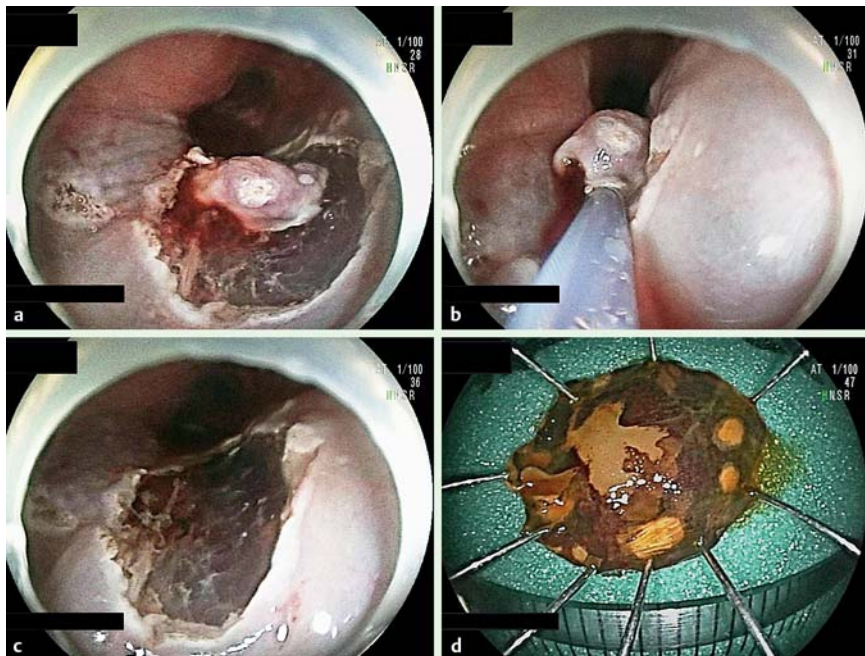


Fig. 4 Completion of endoscopic submucosal dissection using a transnasal endoscope with Nano-shooter hood. **a** The incision around the lesion was completed. **b** A snare was used to resect the lesion. **c** The cancer was completely resected. **d** Resected esophageal cancer.

References

- 1 Nakamura M, Shiroeda H, Tahara T et al. New attachment hood (Nanosooter) for trans-nasal ESD of the hypopharynx. *Endoscopy* 2013; 45 (Suppl. 02): E387–E388
- 2 Yamamoto H, Koiwai H, Yube T et al. A successful single-step endoscopic resection of a 40 millimeter flat-elevated tumor in the rectum, endoscopic mucosal resection using sodium hyaluronate. *Gastrointest Endosc* 1999; 50: 701–704

Bibliography

DOI <http://dx.doi.org/10.1055/s-0034-1364885>
Endoscopy 2014; 46: E115–E116
 © Georg Thieme Verlag KG
 Stuttgart · New York
 ISSN 0013-726X

Corresponding author

Tomiyasu Arisawa, PhD, MD
 Department of Gastroenterology
 Kanazawa Medical University
 1-1, Daigaku
 Uchinada-machi
 Ishikawa 920-0293
 Japan
 Fax: +81-76-2860892
 tarisawa@kanazawa-med.ac.jp