

Partially insulated cutting instruments for hybrid endoscopic submucosal dissection – the Flat Adenoma Resection Instruments (FARIn)

The endoscopic resection of colorectal polyps that are limited to the mucosa is a well established procedure. Nevertheless, modern imaging technology and screening programs have increased the detection of benign but large (>20 mm) polyps.

In flat laterally spreading tumors (LST), especially the nongranular (NG) type, the rate of submucosal invasion is found to be as high as 39% (34%–44%) [1]. For this reason a resection in one piece is mandatory [2].

We report on the resection of a 25-mm flat rectal LST-NG in a 60-year-old patient who was admitted to the Klinikum Augsburg after screening colonoscopy (Fig. 1). Examination with a high definition colonoscope (CF-HQ 190I; Olympus Medical Systems, Tokyo, Japan) demonstrated a Sano Type II, pit pattern IIIs lesion.

We decided to use two newly developed devices, the Flat Adenoma Resection Instruments (Endox-Feinmechanik GmbH, Bad Urach, Germany). Submucosal injection was performed using a mixture of saline, epinephrine (1 : 100 000), glycerol



Fig. 1 Rectal laterally spreading tumor – nongranular type. **a** The tumor during screening colonoscopy. **b** Narrow-band imaging with a high definition colonoscope demonstrated a Sano Type II lesion. **c** After spray application of indigo carmine solution, a surface pit pattern IIIs was diagnosed.


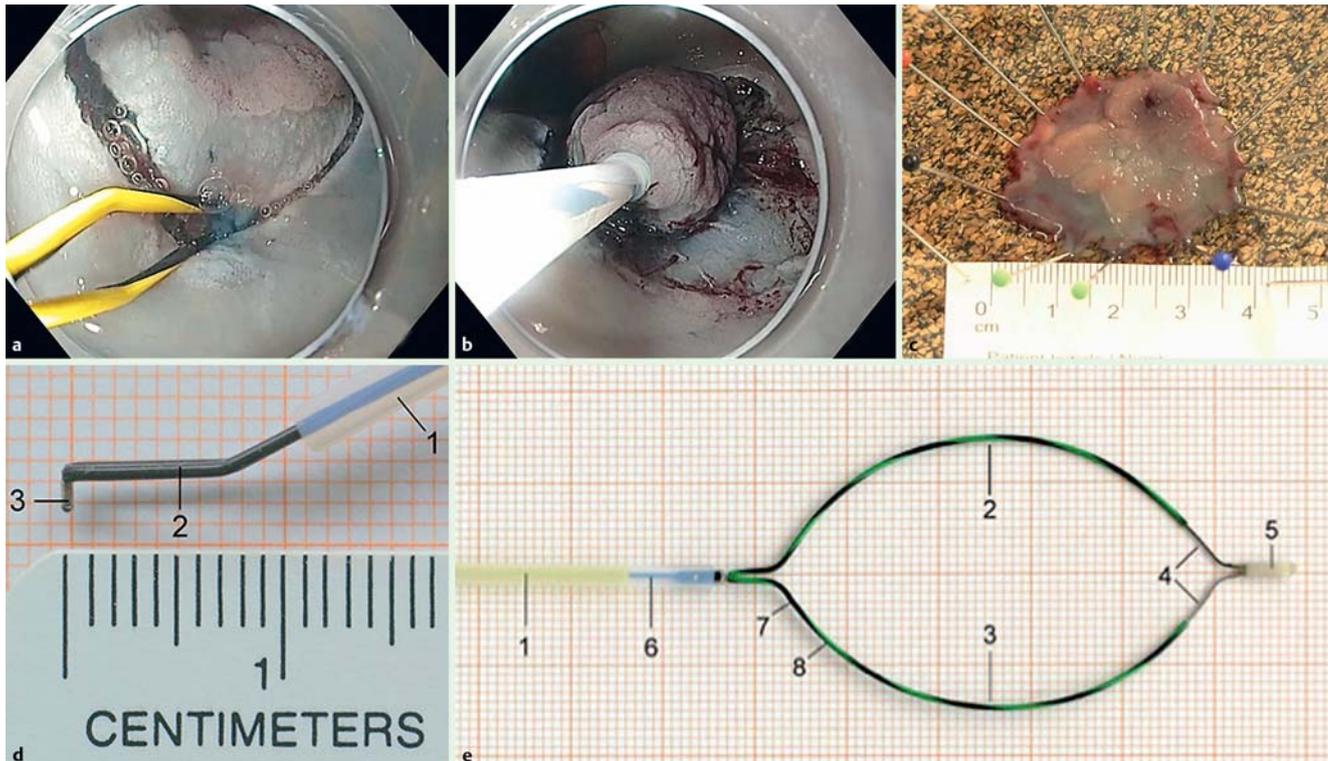


Fig. 2 Resection of the rectal tumor using the Flat Adenoma Resection Instruments (FARIn; Endox-Feinmechanik GmbH, Bad Urach, Germany). **a, d** Hybrid endoscopic submucosal dissection using the FARIn Type I: 1 = catheter sheath; 2 = the rhomboid-shaped and electrically isolated section; 3 = the 1-mm tooth at the distal end, used for circular incision (**a**). **b, e** The specimen could be resected using the partially insulated snare (FARIn Type C): 1 = catheter sheath; 2, 3 = electrically isolated section of the device; 4 = the 15-mm cutting wire at the distal tip of the snare; 5 = the tip of the snare is isolated in order to protect the organ wall from injury; 7, 8 = The colored markings on the snare allow the cutting speed to be visualized when the snare is closed. **c** Resected specimen mounted onto cork, showing the adenoma in the center of the mucosa.

Video 1

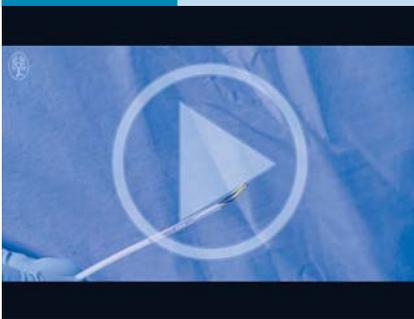

Partially insulated instruments for hybrid endoscopic submucosal dissection of a rectal laterally spreading tumor–nongranular type.

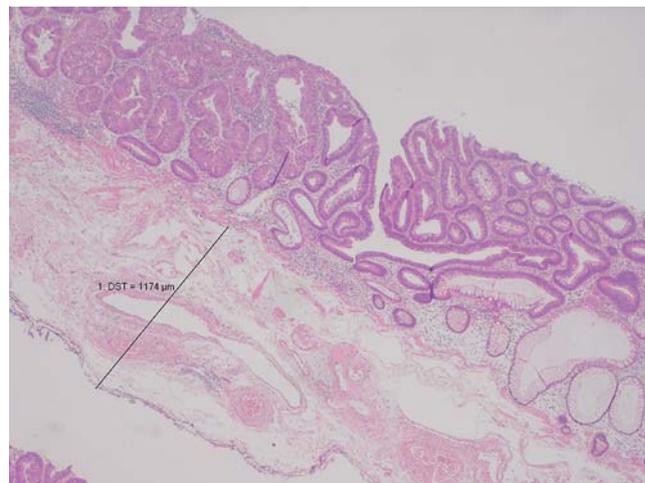


Fig. 3 The histopathological examination showed an adenoma with high grade dysplasia in the center of the lesion and an adherent submucosal layer of $>1000\mu\text{m}$ in depth (DST). Complete (R0) circumferential resection of the lesion was achieved (hematoxylin and eosin $\times 20$).

(10%), and a small amount of indigo carmine solution. Circumferential incision was performed using the FARIn Type I, a rhomboid-shaped device with a small 1-mm cutting tooth at the distal tip. A high frequency generator (VIO 300 D; Erbe, Tübingen, Germany) was configured to AUTO CUT 300W and FORCED COAG 30W. After circumferential incision, the specimen could be resected en bloc using the FARIn Type C, a symmetric snare with a cutting wire length of 15 mm (• Fig. 2, • Video 1).

The histopathological examination showed an adenoma with high grade dysplasia, and an adherent submucosal layer to a depth of $>1000\mu\text{m}$ under the entire lesion (• Fig. 3).

In summary, the FARIn instruments allowed the en bloc resection of a large ($>20\text{mm}$) LST-NG with adherent submucosal layer ($>1000\mu\text{m}$), which meets the specimen requirements for pathological complete resection (R0).

Endoscopy_UCTN_Code_TTT_1AQ_2AD

Competing interests: Dr. Farin is the inventor of the FARIn devices.

Stefan K. Gölder¹, Tina Schaller², Guenter Farin³, Helmut Messmann¹, Andreas Probst¹

¹ Department of Internal Medicine III, Klinikum Augsburg, Augsburg, Germany

² Institute of Pathology, Klinikum Augsburg, Augsburg, Germany

³ FARIN Research, Tübingen, Germany

References

- 1 Yamada M, Saito Y, Sakamoto T et al. Endoscopic predictors of deep submucosal invasion in colorectal laterally spreading tumors. *Endoscopy* 2016; 48: 456–464
- 2 Pimentel-Nunes P, Dinis-Ribeiro M, Ponchon T et al. Endoscopic submucosal dissection: European Society of Gastrointestinal Endoscopy (ESGE) guideline. *Endoscopy* 2015; 47: 829–854

Bibliography

DOI <http://dx.doi.org/10.1055/s-0042-109058>
Endoscopy 2016; 48: E218–E219
 © Georg Thieme Verlag KG
 Stuttgart · New York
 ISSN 0013-726X

Corresponding author

Stefan K. Gölder, MD
 Department of Internal Medicine III
 Klinikum Augsburg
 86156 Augsburg
 Germany
 Fax: +49-821-4003331
stefan.goelder@klinikum-augsburg.de