




Feasibility of performing esophageal endoscopic submucosal dissection using master and slave transluminal endoscopic robot

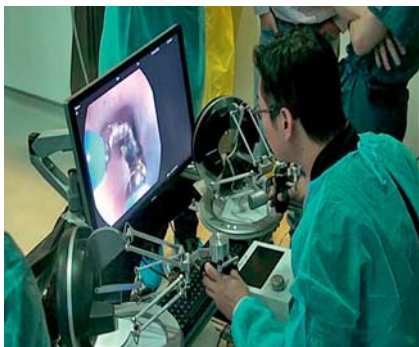

► **Fig. 1** Esophageal endoscopic submucosal dissection (ESD) being performed using the newly developed MASTER endoscopic platform.

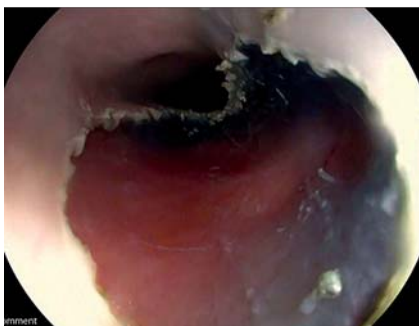

► **Fig. 2** Endoscopic view of the post-endoscopic submucosal dissection (ESD) ulcer.

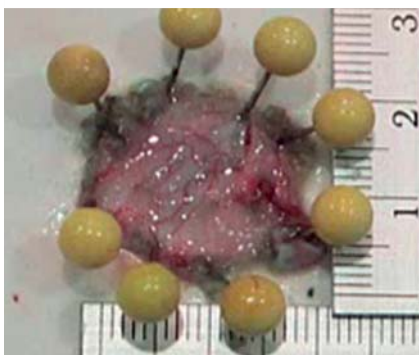

► **Fig. 3** The resected specimen, which measured 20 × 20 mm.

The feasibility of endoscopic submucosal dissection (ESD) using the master and slave transluminal endoscopic robot (MASTER) has been shown in our previous studies [1–3]. Compared with gastric ESD, esophageal ESD remains challenging because of technical difficulties and risks [4, 5]. The aim of this study was to evaluate the feasibility of using MASTER to perform esophageal ESD.

The new version of MASTER was used for esophageal ESD on one pig. The MASTER was redesigned to facilitate performance of ESD within a narrow working space. The main outcomes were: operating time, completeness of resection, and adverse events. The secondary outcomes included: clearance of operative field and limitation of robot arm manipulation in the narrow working space, assessed by counting the number of episodes of blind cutting. For the purpose of comparison with esophageal ESD, one gastric and one colonic ESD were performed by the same operator.

All procedures were successfully completed (► **Table 1**; ► **Figs. 1–3**; ► **Video 1**). It took 15, 63, and 45 minutes to complete the esophageal, gastric, and colonic ESDs, respectively. All lesions were excised en bloc; the specimen sizes were: 20 × 20, 50 × 45, and 35 × 35 mm, respectively. The dissection speeds were: 20.9, 28.0, and 21.4 mm²/min, respectively. There were no adverse events. The number of episodes of blind cutting were: 2, 6, and 6 (0.13, 0.10, and 0.13/min). In contrast to gastric and colonic ESD, the traction of the grasper during esophageal ESD tended to align with the long axis because of the narrow working space. There was no difference comparing esophageal against gastric and colonic ESD in terms of the speed of dissection, the rate of complete resection, the occurrence of adverse events, and the number of episodes of blind cutting. In conclusion, performing esophageal ESD using the MASTER was feasible with a certain degree of adjustment for the narrow working space.

► VIDEO 1



► **Video 1:** Esophageal endoscopic submucosal dissection (ESD) being performed. After marking and injections had been performed, the proximal mucosal incision was created. The mucosa was lifted by the grasper and the submucosa was dissected in parallel with circumferential mucosal cutting. The distal mucosal incision was finally completed and the specimen was resected.

► **Table 1** Outcomes of endoscopic submucosal dissection procedures using the MASTER.

	Procedure 1	Procedure 2	Procedure 3
Organ	Esophagus	Stomach	Colon
Location	Middle thoracic	Middle greater curvature	Sigmoid
Completion	Complete	Complete	Complete
Operation time, minutes	15	63	45
Size of specimen, mm	20×20	50×45	35×35
Dissection speed, mm ² /min	20.9	28	21.4
En bloc/piecemeal	En bloc	En bloc	En bloc
Uncontrolled bleeding	No	No	No
Perforation	No	No	No
Episodes of blind cutting	2	6	6

Endoscopy_UCTN_Code_TTT_1AO_2AG

Competing interests

P.W.Y. Chiu served on the scientific advisory board of EndoMaster Pte Ltd. S.J. Phee and K.Y. Ho are cofounders of EndoMaster Pte Ltd.

The Authors

Nobuyoshi Takeshita¹, Khek Yu Ho², Soo Jay Phee³, Jennie Wong¹, Philip Wai Yan Chiu⁴

- 1 Department of Medicine, National University of Singapore, Singapore
- 2 Yong Loo Lin School of Medicine, National University of Singapore, Singapore
- 3 School of Mechanical and Aerospace Engineering, Nanyang Technological University, Singapore
- 4 Department of Surgery, The Chinese University of Hong Kong, Hong Kong

Corresponding author

Nobuyoshi Takeshita, MD, PhD

Department of Medicine, National University of Singapore, 1E Kent Ridge Road NUHS Tower Block, Level 10 University Medicine Cluster, Singapore 119260, Singapore
 Fax: +65-67724361
 ntakeshita1225@gmail.com

References

- [1] Wang Z, Phee SJ, Lomanto D et al. Endoscopic submucosal dissection of gastric lesions by using a master and slave transluminal endoscopic robot: an animal survival study. *Endoscopy* 2012; 44: 690–694
- [2] Phee SJ, Reddy N, Chiu PW et al. Robot-assisted endoscopic submucosal dissection is effective in treating patients with early-stage gastric neoplasia. *Clin Gastroenterol Hepatol* 2012; 10: 1117–1121
- [3] Ho KY, Phee SJ, Shabbir A et al. Endoscopic submucosal dissection of gastric lesions by using a Master and Slave Transluminal Endoscopic Robot (MASTER). *Gastrointest Endosc* 2010; 72: 593–599
- [4] Tanaka S, Morita Y, Fujita T et al. Ex vivo pig training model for esophageal endoscopic submucosal dissection (ESD) for endoscopists with experience in gastric ESD. *Surg Endosc* 2012; 26: 1579–1586
- [5] Sato H, Inoue H, Ikeda H et al. Clinical experience of esophageal perforation occurring with endoscopic submucosal dissection. *Dis Esophagus* 2014; 27: 617–622

Bibliography

DOI <http://dx.doi.org/10.1055/s-0042-121486>
Endoscopy 2017; 49: E27–E28
 © Georg Thieme Verlag KG
 Stuttgart · New York
 ISSN 0013-726X