



## Successful endoscopic closure of iatrogenic duodenal perforation with the new Padlock Clip

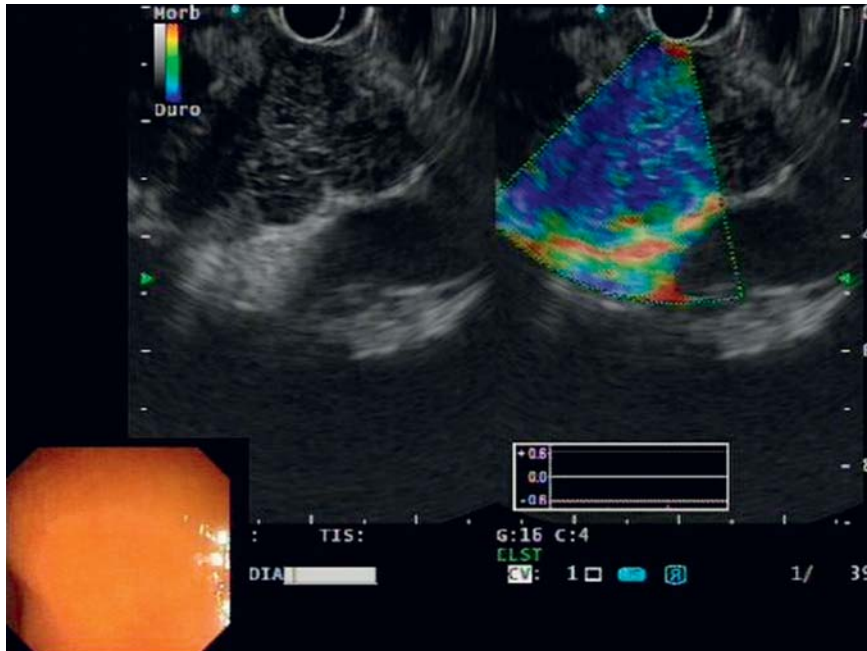

► **Fig. 1** Solid lesion seen in the pancreatic head on endoscopic ultrasound.

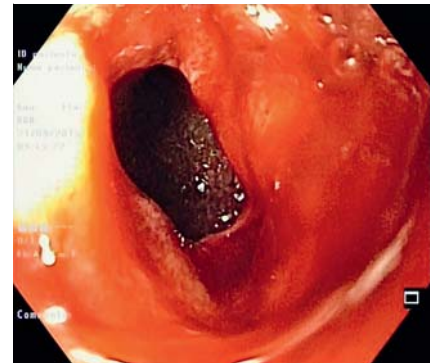

► **Fig. 2** Full-thickness defect at the upper duodenal knee.



► **Fig. 3** The new Padlock Clip (Aponos Medical Co., Kingston, New Hampshire, USA).

Although duodenal perforations are rare [1], they represent one of the most critical complications of endoscopic ultrasound (EUS) and may be fatal in elderly patients. Following the introduction of endoscopic clips, stents, and over-the-scope systems into clinical practice, endoscopic management of perforations has become the first therapeutic option [2, 3].


We present the case of a 62-year-old man with jaundice, who was referred to the Digestive Endoscopy Unit of Humanitas Research Hospital (Rozzano, Italy) to undergo EUS-guided fine-needle aspiration of a solid lesion in the pancreatic head (► **Fig. 1**). The EUS was performed using a linear echoendoscope (GF-UCT140; Olympus Optical Co., Tokyo, Japan), CO<sub>2</sub> insufflation, and with the patient under deep sedation with propofol.

During scope withdrawal through the duodenum, we observed a type-1 [4], full-thickness defect, of 13 mm in diameter, at the upper duodenal knee (► **Fig. 2**).

A stiff guidewire was placed in the duodenum to help expose the defect. A twin grasper (Ovesco Endoscopy AG, Tübingen, Germany) was used to approximate the mucosal edges of the perforation. Then, a gastroscope loaded with the new Padlock Clip (Aponos Medical Co., King-

► **VIDEO 1**

► Video 1: Endoscopic closure of an iatrogenic duodenal perforation using the new Padlock Clip system (Aponos Medical Co., Kingston, New Hampshire, USA).

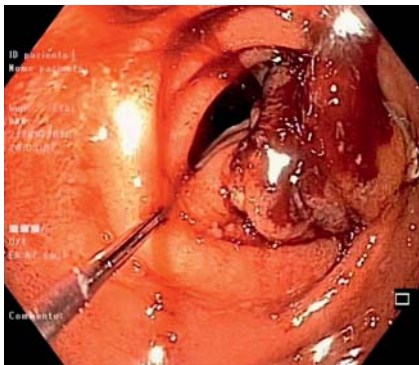

► **Fig. 4** Final endoscopic appearance after deployment of the Padlock Clip (Aponos Medical Co., Kingston, New Hampshire, USA).



► **Fig. 5** Final fluoroscopic appearance of the Padlock Clip (arrow; Aponos Medical Co., Kingston, New Hampshire, USA).

ston, New Hampshire, USA) (► **Fig. 3**) was used to seal the defect (► **Video 1**). Finally, a contrast radiograph confirmed the complete closure of the perforation (► **Fig. 4**, ► **Fig. 5**).

The Padlock Clip is a new over-the-scope system designed to be placed parallel to the endoscope, without occupying the operative working channel [5]. To our knowledge, this is the first clinical experience of closure of a duodenal iatrogenic perforation using the Padlock Clip.

Endoscopy\_UCTN\_Code\_CPL\_1AL\_2AB

### Competing interests

None

### The Authors

**Andrea Anderloni<sup>1</sup>, Mario Bianchetti<sup>2</sup>, Benedetto Mangiavillano<sup>2</sup>, Alessandro Fugazza<sup>1,3</sup>, Milena Di Leo<sup>1</sup>, Silvia Carrara<sup>1</sup>, Alessandro Repici<sup>1,4</sup>**

- 1 Digestive Endoscopy Unit, Division of Gastroenterology, Humanitas Research Hospital, Rozzano, Italy
- 2 Gastrointestinal Endoscopy Unit, Humanitas Mater Domini, Castellanza, Italy
- 3 Digestive Endoscopy Unit, University of Parma, Parma, Italy
- 4 Humanitas University, Rozzano, Italy

### Corresponding author

**Andrea Anderloni, MD, PhD**

Digestive Endoscopy Unit, Division of Gastroenterology, Humanitas Research Hospital, Via Manzoni 56, 20089 Rozzano (Milano), Italy  
 Fax: +39-02-82247308  
 andrea.anderloni@humanitas.it

### References

- [1] Carrara S, Arcidiacono PG, Mezzi G et al. Pancreatic endoscopic ultrasound-guided fine needle aspiration: complication rate and clinical course in a single centre. *Dig Liv Dis* 2010; 42: 520 – 523
- [2] Paspatis GA, Dumonceau JM, Barthet M et al. Diagnosis and management of iatrogenic endoscopic perforations: position statement from the European Society of Gastrointestinal Endoscopy (ESGE). *Endoscopy* 2014; 46: 1 – 19
- [3] Guarner-Argente C, Córdova H, Martínez-Pallí G et al. Yes, we can: reliable colonic closure with the Padlock-G clip in a survival porcine study (with video). *Gastrointest Endosc* 2010; 72: 841 – 844
- [4] Mangiavillano B, Caruso A, Manta R et al. Over-the-scope clips in the treatment of gastrointestinal tract iatrogenic perforation: a multicenter retrospective study and a classification of gastrointestinal tract perforations. *World J Gastrointest Surg* 2016; 8: 315 – 320
- [5] Armellini E, Crinò SF, Orsello M et al. Novel endoscopic over-the-scope clip system. *World J Gastroenterol* 2015; 21: 13587 – 13592

### Bibliography

DOI <http://dx.doi.org/10.1055/s-0042-124177>  
*Endoscopy* 2017; 49: E58–E59  
 © Georg Thieme Verlag KG  
 Stuttgart · New York  
 ISSN 0013-726X