


## Novel wire-guided fine-gauge bougie dilator for transpapillary or endoscopic ultrasonography-guided biliary drainage

Endoscopic management of biliary stricture generally requires dilation using devices such as an endoscopic retrograde cholangiopancreatography (ERCP) balloon dilation catheter before stenting [1]. Endoscopic ultrasonography (EUS)-guided biliary drainage (EUS-BD) also requires fistula dilation before stenting. Recently, ultraslim balloon catheters [1] and diathermic dilators [2] have also been developed as dilation devices. These devices must be wire-guided, coaxial with the guidewire, fine-gauge, and sufficiently stiff.

Herein, we present two patients who successfully underwent biliary dilation using a novel wire-guided fine-gauge bougie dilator (ES dilator soft type; Zeon Medical Inc., Tokyo, Japan) (► **Fig. 1** and ► **Fig. 2**) for transpapillary drainage and EUS-BD.

The first patient was a 79-year-old man who was admitted with obstructive jaundice having undergone placement of self-expandable metal stents (SEMSs) for perihilar bile duct cancer 5 months previously. An ERCP showed occlusion of the SEMSs (► **Fig. 3 a**). First, a 0.025-inch hard-type guidewire (VisiGlide 2; Olympus, Tokyo, Japan) was advanced across the occluded SEMSs. A tapered ERCP catheter and a dilation catheter (SBDC-6; Cook Japan, Tokyo, Japan) could not be passed through the stricture (► **Video 1**). The novel dilator was then inserted, resulting in successful passage through the occluded SEMSs (► **Fig. 3 b**; ► **Video 1**). Finally, an uncovered SEMS was placed without any complications.

The second patient was an 85-year-old man who was admitted with obstructive jaundice and a history of total gastrectomy and Roux-en-Y reconstruction for gastric cancer 21 years previously. A computed tomography (CT) scan showed an ampullary tumor and treatment by EUS-BD was selected. Firstly, B3 was punctured with a 19-gauge needle via the jejunum and a 0.025-inch hard-

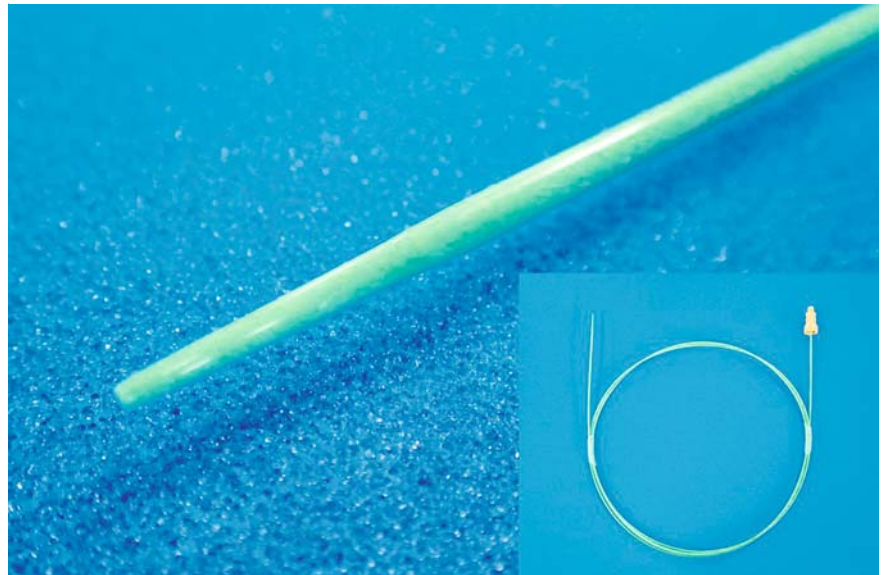


► **Fig. 1** The tip of the novel fine-gauge bougie dilator (ES dilator soft type; Zeon Medical Inc., Tokyo, Japan) is 3.2-Fr in diameter, tapered, and coaxial with the 0.035-inch guidewire, and has a radiopaque marker to help during insertion. Its maximum diameter is 7.4-Fr. Inset: Image of the whole dilator.

type guidewire (VisiGlide 2; Olympus) was placed. A tapered ERCP catheter was tried without success to dilate the fistula. Subsequently, dilation with the

novel dilator was attempted, and this was successfully inserted into the intrahepatic bile duct (► **Fig. 4**; ► **Video 2**). Finally, EUS-guided antegrade stenting

### ► VIDEO 1

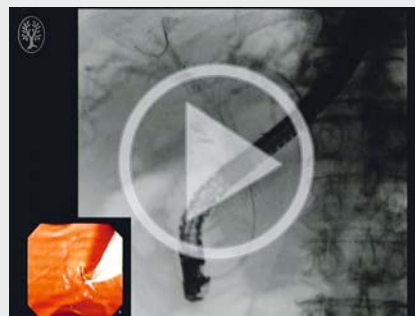

► **Video 1:** Images from patient #1 during endoscopic retrograde cholangiopancreatography showing that a Soehendra biliary dilation catheter could not be passed through the stricture but the ES dilator soft type was easily passed through the stricture. Finally, an uncovered self-expandable metal stent insertion for revision was performed.



► **Fig. 2** The novel fine-gauge bougie dilator (ES dilator soft type; 3.2-Fr tip; Zeon Medical Inc., Tokyo, Japan; right side in all images) is compared with: **a** a conventional bougie dilator (SBDC-6; 4-Fr tip and maximum diameter of 6-Fr; Cook Japan, Tokyo, Japan) shown placed over a 0.035-inch guidewire; **b** an ultraslim balloon catheter (ZARA EPBD balloon; 3.1-Fr tip and maximum diameter of 6.3-Fr; Century Medical Inc., Tokyo, Japan) shown placed over a 0.035-inch guidewire; **c** an ultraslim balloon catheter (REN biliary dilation catheter; 3-Fr tip and maximum diameter of 6.4-Fr; Kaneka Corporation, Osaka, Japan) shown placed over a 0.025-inch guidewire. The ES dilator and ZARA EPBD balloon are excellent for having minimal difference in caliber between the guidewire and the catheter.

was performed without any complications (► **Video 2**).

The novel wire-guided fine-gauge bougie dilator is useful for both transpapillary and fistula dilation in EUS-BD owing to its ideal thickness and stiffness.


Endoscopy\_UCTN\_Code\_TTT\_1AS\_2AD

### Competing interests


The novel bougie dilator has been developed through collaborative research between Dr. Kawakami and Zeon Medical Inc., Tokyo, Japan. Dr. Kawakami is a consultant and gives lectures for the Zeon Medical Inc. The authors declare no conflict of interests for this article.

► **VIDEO 2**

► **Video 2:** Images from patient #2 during endoscopic ultrasonography (EUS)-guided biliary drainage showing a guidewire placed in the intrahepatic bile duct after puncture of B3 with a 19-gauge needle. A tapered endoscopic retrograde cholangiopancreatography (ERCP) catheter could not be passed through the stricture; however, the ES dilator soft type was inserted with ease. It was then possible to pass a tapered ERCP catheter through the distal biliary stricture and finally EUS-guided antegrade stenting was performed for the distal biliary obstruction.

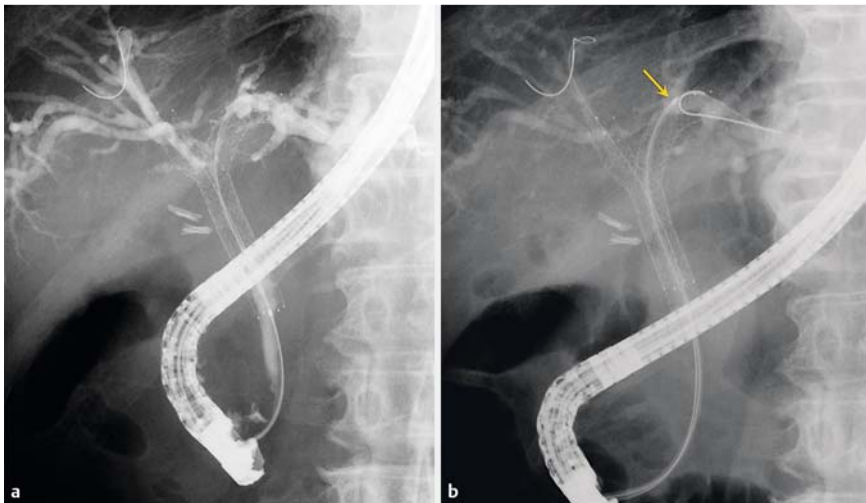

► **Fig. 3** Radiographic images from patient #1 showing: **a** recurrent perihilar biliary obstruction after multistenting in a stent-in-stent fashion; **b** the ES dilator soft type (arrow) that has been passed through the refractory biliary stricture.

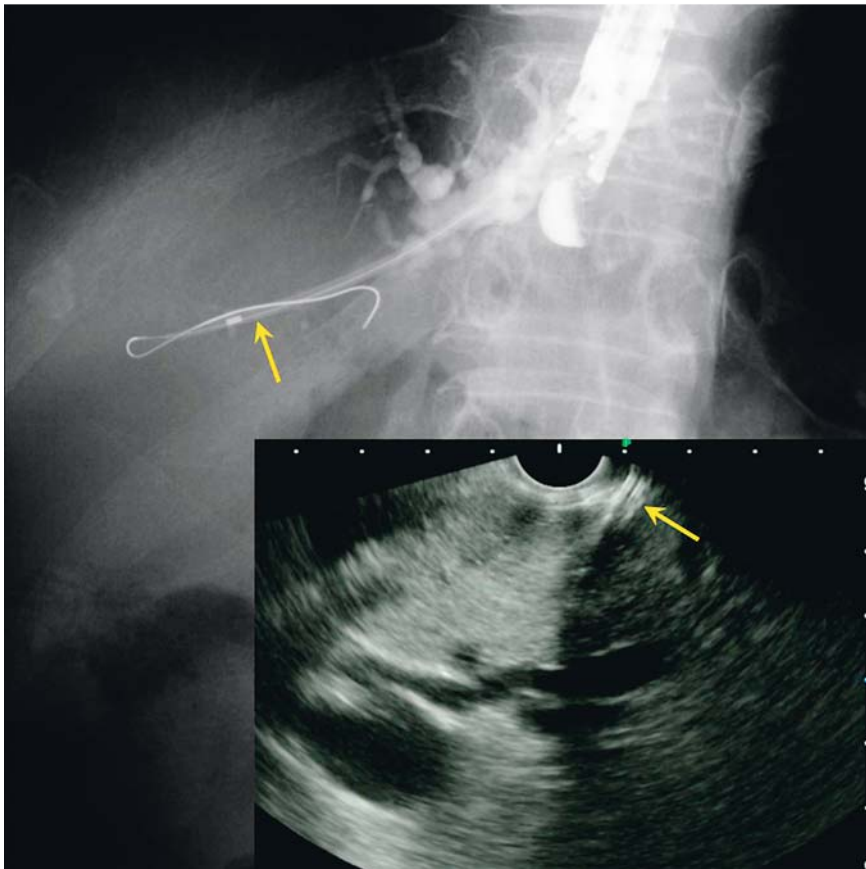

► **Fig. 4** Radiographic image from patient #2 showing the ES dilator soft type (arrow) that was successfully advanced through the jejunal wall and intrahepatic bile duct after a failed attempt at fistula dilation using a tapered endoscopic retrograde cholangiopancreatography catheter. Inset: Endoscopic ultrasonography view showing the ES dilator soft type (arrow).

## The Authors

**Hiroshi Kawakami, Yoshimasa Kubota**  
 Department of Gastroenterology and  
 Hepatology, University of Miyazaki and Center  
 for Digestive Disease, University of Miyazaki  
 Hospital, Miyazaki, Japan

## Corresponding author

**Hiroshi Kawakami, MD, PhD**  
 Department of Gastroenterology and  
 Hepatology, University of Miyazaki,  
 Center for Digestive Disease, University of  
 Miyazaki Hospital, 5200, Kihara, Kiyotake,  
 Miyazaki 889-1692, Japan  
 Fax: +81-985-859802  
 hiropon@med.miyazaki-u.ac.jp

## References

- [1] Kawakami H, Kuwatani M, Kawakubo K et al. Transpapillary dilation of refractory severe biliary stricture or main pancreatic duct by using a wire-guided diathermic dilator (with video). *Gastrointest Endosc* 2014; 79: 1–3
- [2] Ogura T, Takagi W, Onda S et al. Endoscopic ultrasound-guided biliary drainage with a novel fine-gauge balloon catheter: simplified technique using a coaxial guidewire. *Endoscopy* 2015; 47: E573–E574

## Bibliography

DOI <http://dx.doi.org/10.1055/s-0042-124498>  
*Endoscopy* 2017; 49: E75–E77  
 © Georg Thieme Verlag KG  
 Stuttgart · New York  
 ISSN 0013-726X