



Endocuff Vision to Improve Adenoma Vision: A Brief Overview

Jayendra Shukla¹ Jayanta Samanta¹

¹Department of Gastroenterology, Postgraduate Institute of Medical Education and Research, Chandigarh, India

Address for correspondence Jayanta Samanta, MD, DM, Department of Gastroenterology, Post Graduate Institute of Medical Education and Research, Chandigarh, Sector 12, Chandigarh 160012, India (e-mail: dj_samanta@yahoo.co.in).

J Digest Endosc 2022;13:193–198.

Abstract

Colorectal cancer (CRC)-related mortality can be reduced through screening and early detection. The aim of any CRC screening program is to detect as many adenomas/polyps in the early stage as possible and hence, adenoma detection rate (ADR) is a key quality indicator of colonoscopy. Various methods and techniques have been studied and developed over the years to improve the quality of colonoscopy and thereby increase ADR. This ranges from use of various regimens to improve bowel preparation, defining an optimum colonoscope withdrawal time for the operator, distal attachment caps, use of different wavelength of light, colonoscope with increased degree of view to the use of modern-day artificial intelligence to improve ADR. Of all the various measures, use of distal attachment device seems an easy, cheap and readily usable technique to increase real-time ADR. A variety of such devices have been evaluated over time starting from simple transparent caps, EndoRings, Endocuff to Endocuff Vision for their effectiveness. In this review, we have provided a brief description of the various available distal attachment devices and a detailed technical overview of Endocuff and its modification the Endocuff Vision.

Keywords

- ▶ colonoscopy
- ▶ polyp
- ▶ adenoma detection rate
- ▶ distal attachment cap
- ▶ colorectal cancer

Introduction

Colonoscopy has been the procedure of choice for polyp/adenoma detection for quite some time now. It helps decrease interval colorectal cancers¹, although its diagnostic efficacy is affected by a host of factors. A good preparation, adequate time for withdrawal, operator expertise, and a high-definition scope are some of the prerequisites for obtaining an acceptable adenoma detection rate (ADR). As demonstrated by Corley et al, ADR is a critical factor in preventing interval colon cancer² and hence is considered as the primary quality indicator of colonoscopy. The optimal ADR should be at least 20% for centers that run a bowel cancer screening program. Various modifications have been implemented and evaluated over the

ensuing years to improve ADR. We can achieve this by either using some attachment device at the tip of the colonoscope to increase visual field, use different light wavelengths (narrow band imaging and chromoendoscopy), employ artificial intelligence or by using a scope with a better 360 degrees view (full sense colonoscope).³ Of all the various measures, use of distal attachment device seems an easy, cheap and readily usable technique to increase real-time ADR. Most of the polyps that are missed are usually behind the folds, haustra or hidden around flexures. The attachment devices are meant to address this lacuna of a standard colonoscopy by stretching out every corner of the colonic mucosa to unfold a hidden polyp. The attachment devices that are currently available include simple transparent caps, Endo-rings and Endocuff.⁴ We, in this review,

DOI <https://doi.org/10.1055/s-0042-1755338>.
ISSN 0976-5042.

© 2022. Society of Gastrointestinal Endoscopy of India. All rights reserved.

This is an open access article published by Thieme under the terms of the Creative Commons Attribution-NonDerivative-NonCommercial-License, permitting copying and reproduction so long as the original work is given appropriate credit. Contents may not be used for commercial purposes, or adapted, remixed, transformed or built upon. (<https://creativecommons.org/licenses/by-nc-nd/4.0/>)

Thieme Medical and Scientific Publishers Pvt. Ltd., A-12, 2nd Floor, Sector 2, Noida-201301 UP, India

aim to give a brief description of the various available distal attachment devices and a detailed technical overview of Endocuff and its modification the Endocuff Vision.

Available Distal Attachments and Their Mechanism of Action

A host of different distal attachment devices are available of which the most used are transparent cap, EndoRings, and Endocuff. ► **Table 1** gives a comparative summary of these various devices.

Transparent Cap

The most commonly used attachment device is the standard transparent cap which is easily available and is mostly used for therapeutic procedures to improve visualization. It separates the endoscope tip and thus, the lens of the scope from the mucosa or area of interest by a working distance of usually around 4 mm. This facilitates optimum visualization of the target area without experiencing “red-out.” The various available transparent caps manufactured by different companies (Steris Healthcare, Dublin, Ireland; Olympus Medical, Tokyo, Japan; Finemedix, Seoul, Korea; Synectics Medical Ltd., Enfield, United Kingdom) have almost similar design.

Mir et al, in their meta-analysis, compared cap-assisted colonoscopy (CAC) with standard colonoscopy (SC) and found that CAC showed statistically significant superiority in total colonoscopy time ($p < 0.01$) and time to cecum ($p < 0.01$) compared with SC. CAC also showed better polyp detection rate (PDR) ($p < 0.01$) but not ADR ($p = 0.20$). Though on sensitivity analysis, ADR was better with CAC; terminal ileum intubation and cecal intubation rates were similar between the two groups ($p = 0.11$ and $p = 0.73$, respectively).⁵ Thus, transparent cap is an easy-to-use, cheap tool and can help enhance the PDR.

EndoRings

EndoRings (EndoAid Ltd, Caesarea, Israel) comprises of flexible silicone rings that are attached in three circular rows around the distal end of the colonoscope. They improve

visualization of colonic mucosa by mechanically straightening colonic folds during withdrawal and by keeping the tip of colonoscope in the center of the lumen. The CLEVER study, comparing EndoRings with SC in a randomized controlled trial, demonstrated that EndoRings had significantly lower adenoma (10.4 vs. 48.3%; $p < 0.0001$) and polyp miss rates (9.1 vs. 52.8%; $p < 0.0001$) than SC, with similar cecal intubation and withdrawal times.⁶ However, a similar study, the SMART trial failed to demonstrate any advantage of EndoRings over SC.⁷ With two studies exhibiting contradicting data, the role of EndoRings in the enhanced polyp detection strategy needs to be still established.

Endocuff

Endocuff (Arc Medical Design, Leeds, United Kingdom) is a device made of a plastic barrel with two rows of thermo-plastic elastomer spikes. This device is attached to the tip of the colonoscope, and the spikes are used to flatten the mucosal folds during withdrawal. This can enable visualization of the polyps on the reverse side of the mucosal folds and increase right-sided ADRs.


Triantafyllou et al⁸, in a multicenter RCT, showed that Endocuff-assisted colonoscopy had significantly lower overall and proximal colon adenoma miss rates compared with conventional colonoscopy (14.7 vs. 38.4% and 10.4 vs. 38.9%, respectively). Though revolutionary in design, Endocuff has been described to have a few drawbacks including mucosal lacerations and erosions and difficulty in terminal ileum intubation. This paved the path for its congener, namely Endocuff Vision.

Endocuff Vision

The new, second generation Endocuff Vision (ECV), from Olympus, has some modifications over the older version as is depicted in ► **Fig. 1**. Compared with the first-generation device, the ECV has only one row of flexible arms that are softer and 2 mm longer (► **Fig. 2**). The new design is a single-use device that is made of a polypropylene cylinder with a

Table 1 Distal attachment devices

Device	Distal attachment cap	Endocuff	Endocuff Vision	EndoRings
Manufacturer	Olympus, Centre Valley, Pennsylvania 1993	Arc Medical Leeds, United Kingdom 2011	Olympus Medical, Tokyo, Japan and Arc Medical Leeds, United Kingdom, 2016	EndoAid Ltd, Caesarea, Israel, 2015
Mode of action	Protruding cap manipulates and flattens haustral folds to inspect the mucosa on the proximal side of the fold maintaining optimal field of view	Hinged projections flatten and spread mucosa and folds	Hinged projections flatten and improve visibility behind the colon folds	Sequential rings stretch out the folds of the colon during withdrawal for a clear view
Disadvantages	Interfere with the field of view	Petechial marks on colon; Potential dislodgement; Larger model more effective than smaller; Ileum intubation may be difficult	Potential dislodgement	Ileum intubation may be difficult

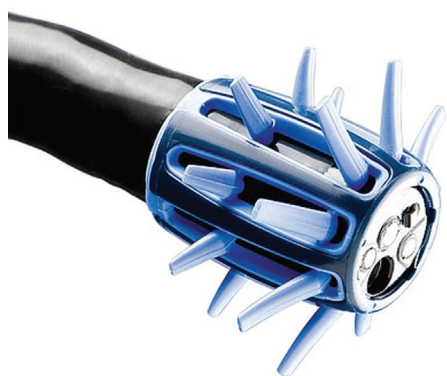

A



B

Fig. 1 (A) Endocuff; (B) Endocuff Vision. Source: <https://www.red-dot.org/project/endocuff-27518>

single row of eight spikes, longer than in the first generation Endocuff. There are four different color-coded sizes to fit in all scopes ranging from adult to pediatric ones (►Table 2). ECV is mounted at the tip of a colonoscope in the same way as the earlier version (►Fig. 2). Its spikes fold back while inserting the scope in the colon as there is a small hinge at

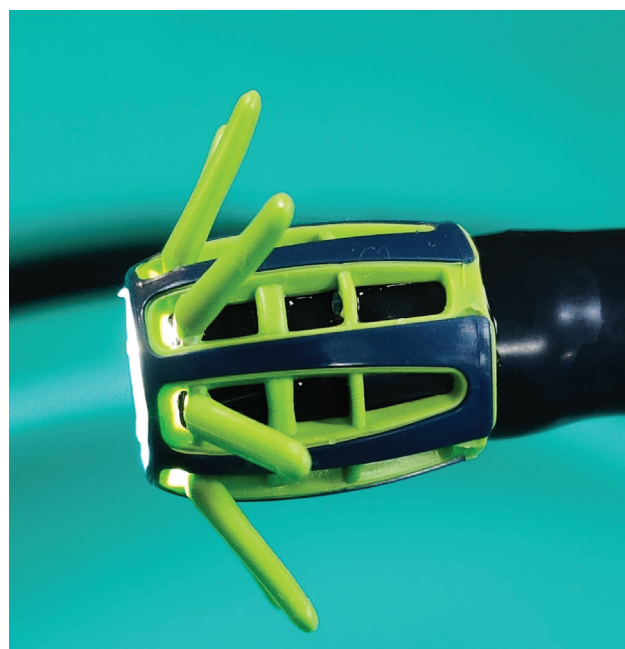


Fig. 2 Endocuff Vision mounted on the tip of a standard colonoscope: single row of spikes.

the base of each spike. They help hold on to a fold and reduce the scope in case of a loop formation. It helps in early and controlled view of the upstream surface of the large colonic folds in the right colon and prevents sudden scope slip-back. This property also makes it easier for polypectomy by stabilizing the scope. After cecal intubation these spikes evert while coming back and increase the mucosal exposure with visualization behind the folds (►Fig. 3). Moreover, when in the sigmoid colon, the device facilitates the opening of contracted folds, permitting a clearer view of the in-between mucosa.

Is Endocuff Vision Better than the Original Endocuff?

Modifications of devices are aimed to improve the efficacy and reduce the adverse effects. For ECV, the data are still emerging as to whether one row is better than two. A recent network meta-analysis of 12 RCTs showed that while

Table 2 Endocuff Vision sizes and compatible scopes

Catalog number	Color	Size	Diameter (mm)	Compatible scopes
ARV110	Blue	Medium	11.0	PCF-H190DL/I
ARV120	Green	Large	11.2	CF-HQ190L/I, CF-Q180AL/I, CF-H180AL/I, CF-160 series, CF-1T 140L
ARV130	Purple	Small	10.4	PCF-H190L/I, PCF-H180AL/I, PCF-Q180, PCF-160 series
ARV140	Orange	Extra large	12.1	CF-H180DL/I

Source: <https://medical.olympusamerica.com/products/endocuffvision>.

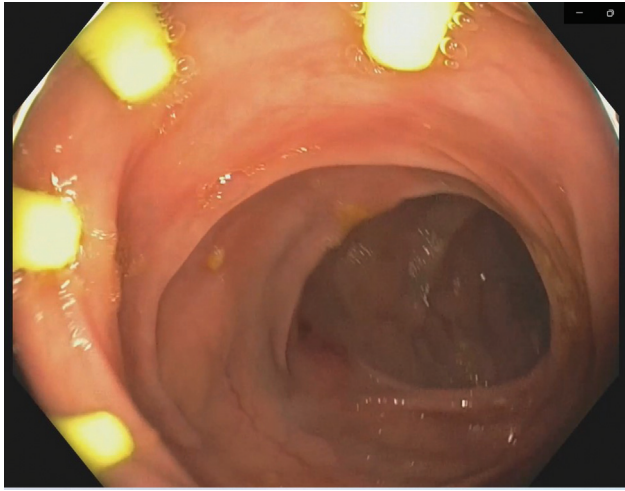


Fig. 3 Eversion of the spikes noted during withdrawal in colonoscopy to flatten the folds.

Endocuff had better ADR compared with high-definition colonoscopy (RR: 1.26; 95% CI 1.09–1.46), the same was not true for ECV (RR: 1.12; 95% CI 0.99–1.27).⁹ The overall complication rates, specially lacerations/erosions were lower with ECV. While Endocuff seemed to fare better on ADR, ECV probably has a better safety profile. However, none of these studies had studied the two congeners head-to-head and thus, such trials are needed to answer this question better.

Does Endocuff Vision Score over Standard Colonoscopy?

Patel et al in their meta-analysis of eight RCTs comparing ECV with standard colonoscopy (SC) included 5,695 patients and in the final analysis, 2,862 patients (mean age, 62.8 years; 52.9% men) in the ECV group and 2,833 patients (mean age, 62.6 years; 54.2% men) in the SC group. Compared with SC, use of ECV was associated with a significant improvement in ADR (49.8 vs. 45.6%, respectively; RR, 1.12; $p = 0.02$), PDR (58.1 vs. 53%, respectively; RR, 1.12; $p = 0.009$), and adenoma per colonoscopy ($p < 0.01$). Furthermore, use of ECV had a

0.93 minute lower mean withdrawal time ($p < 0.01$) when compared with SC. The difference in ADR was larger in the screening/surveillance population (6.5%, $p = 0.02$) and when used by endoscopists with ADRs $< 30\%$ (9.4%, $p = 0.03$).¹⁰

The ADENOMA trial by Ngu et al¹¹ demonstrated that ECV improved ADR from 36.2 to 40.9% ($p = 0.02$). ECV patients had higher detection of mean adenomas per procedure, sessile serrated polyps, left-sided, diminutive, small adenomas and cancers (cancer 4.1 vs. 2.3%, $p = 0.02$). Rees et al¹², in the B ADENOMA study, however did not find any significant difference due to ECV in ADR or PDR. A synopsis of the various RCTs using ECV in terms of ADR has been outlined in ►Table 3. Overall, ECV seemed to score over SC in terms of ADR and hence, can prove to be beneficial.

Performance of Endocuff in Various Technical Aspects

While ADR is the primary outcome assessed in any study using Endocuff, various other technical outcomes have also been reported. Rex et al¹³ demonstrated that mean insertion time with Endocuff was 4.0 minutes compared with 4.4 minutes for SC ($p = 0.14$). Mean withdrawal time with Endocuff was 6.5 minutes compared with 8.4 minutes for SC ($p < 0.0001$).

Jacob et al¹⁴ in their RCT found out that PDP was significantly higher in ECV group than SC (53% in the ECV group vs. 41.1% in SC, $p = 0.035$). However, no statistical difference was noted in terms of polyp site detection. The independent predictors of polyp detection were use of ECV, age > 60 years, and withdrawal time. No complications were reported in their study and showed that if right size was used the dislodgement rate was negligible.

The ADENOMA trial¹¹ showed that the median intubation time was a minute faster with ECV ($p = 0.001$), but had no difference in cecal intubation rate or withdrawal time. ECV exhibited minor increase in discomfort on anal intubation with no or minimal sedation with an ECV removal rate of 4.1%. Thus, while conflicting data exist on the performance of ECV over SC in terms of cecal intubation or withdrawal time, the former performs better as far as PDR is concerned.

Table 3 Randomized controlled trials using Endocuff Vision

Author	Year	Country	Patients (ECV/Comparator)	Comparison arm	Results (ECV/Comparator)
Rex et al ¹³	2020	United States	101/99	Standard colonoscopy	ADR (61.4 vs. 52%; $p = 0.21$)
Jacob et al ¹⁴	2018	Australia	182/138	Standard colonoscopy	ADR (36.8 vs. 28.9%; $p =$ not significant)
Figura et al ¹⁸	2019	Germany	118/122	Standard colonoscopy	ADR (38.1 vs. 42.6%, respectively; $p = 0.48$)
Ngu et al ¹¹	2017	United Kingdom	888/884	Standard colonoscopy	ADR (40.9 vs. 36.2%, respectively; $p = 0.02$)
Karsenti et al ¹⁹	2019	France	1,026/1,032	Standard colonoscopy	ADR (39.2 vs. 29.4%, respectively; $p = 0.001$)
Rees et al ¹²	2019	United Kingdom	1,610/1,612	Standard colonoscopy	ADR (13.3 vs. 12.2%, respectively; $p = 0.35$)

Abbreviations: ADR, adenoma detection rate; ECV, Endocuff Vision.

Comparison with Other Distal Attachment Devices

In the DETECT trial, by Rameshshanker R et al,¹⁵ polyp miss rate was significantly lower in ECV (8.4%) as compared with CAC (26.1%, $p < 0.001$). Similar results were deduced for adenoma miss rate (ECV vs. CAC, 6 vs. 19%; $p = 0.002$) and diminutive adenoma (<5 mm) miss rate in the ECV group (1.8 vs. 19.6%, $p < 0.001$). However, there were no significant differences in the miss rates for small adenomas (5–9 mm) (3.7 vs. 2.9%, $p = 0.69$) or adenomas 10 mm or larger (1.6 vs. 2.6%, $p = 0.98$). The mean number of adenomas per procedure was significantly higher with ECV compared with CAC (1.5 vs. 0.8, $p < 0.001$). Cecal intubation time was significantly shorter with ECV than CAC (median 6 vs. 7 minutes, $p = 0.01$). However, withdrawal time (median 10 vs. 8 minutes, $p = 0.01$) was significantly longer in ECV.

Marsano et al¹⁶ also looked at the benefit of different capped devices. They performed a randomized controlled trial looking at the ECV, transparent cap from Olympus, and conventional colonoscopy. In this study, the ADR of ECV stood out again with 54 versus 52% for conventional colonoscopy. Interestingly, they found that the transparent cap on ADR was of just 40%.

Overall, ECV showed slight benefit over other distal attachment devices in terms of ADR, probably more for diminutive polyps.

Caveats of the Device

The device makes the colonoscope tip wider than usual which may lead to painful anal intubation and the widened tip with the plastic fingers renders ileal intubation difficult. While no specific tip or trick has been outlined in literature, different authors have shared their experience that ileal intubation is difficult with an Endocuff device. In the authors' experience too, it was difficult to intubate the ileum. The purpose of this device is to see behind folds so that polyps are not missed in colon, ileal intubation may not be warranted while using ECV. Dislodgment can be an issue (removal rate 4.1%)¹¹ but it is rarely seen due to dry grip of plastic barrel over colonoscope tip.

AmplifEYE: Similar Looking Device

A device akin to ECV, with a single row of detection arms, is the AmplifEYE device (Medivators, Minneapolis, Minnesota, United States) which is less expensive. Both are U.S. FDA approved. In fact, a head-to-head trial, by Rex et al,¹⁷ showed that both had similar ADR.

Conclusion

Overall, Endocuff, both the original and/or the newer version Vision, seems promising in enhancing ADR. It has performed better than SC alone or sometimes with other attachment devices. Multiple randomized controlled trials have been undertaken and the ADENOMA and DETECT studies are significant in this context. It is an affordable device and easy to use. Whether the single row of ECV is more efficacious than the older Endocuff is debatable, although ECV

does have lower complication rates. The shortcomings include painful anal intubation, difficult ileal intubation, and a small dislodgement risk. However, more data are required before it can be recommended for regular use. In India, with the lack of a systematic bowel cancer screening program, experience with this attachment device is limited to some tertiary care centers alone. However, considering the simplicity and easy availability of the device, it may be advocated for more and more use in centers engaged with screening colonoscopies.

Authors' Contributions

J.S. contributed toward conception and design, review of literature, data analysis, drafting the work, and final approval. J.S. did the conception and design, data interpretation, intellectual review of the work, and final approval. All the authors have approved the final version of the work.

Funding

None.

Conflict of Interest

None declared.

References

- Gkolfakis P, Tziatzios G, Spartalis E, Papanikolaou IS, Triantafyllou K. Colonoscopy attachments for the detection of precancerous lesions during colonoscopy: a review of the literature. *World J Gastroenterol* 2018;24(37):4243–4253
- Corley DA, Jensen CD, Marks AR, et al. Adenoma detection rate and risk of colorectal cancer and death. *N Engl J Med* 2014;370(14):1298–1306
- Zippi M, Hong W, Crispino P, Traversa G. New device to implement the adenoma detection rate. *World J Clin Cases* 2017;5(07):258–263
- Zorzi M, Hassan C, Battagello J, et al; ItaVision Working Group. Adenoma detection by Endocuff-assisted versus standard colonoscopy in an organized screening program: the "ItaVision" randomized controlled trial. *Endoscopy* 2022;54(02):138–147
- Mir FA, Boumitri C, Ashraf I, et al. Cap-assisted colonoscopy versus standard colonoscopy: is the cap beneficial? A meta-analysis of randomized controlled trials. *Ann Gastroenterol* 2017;30(06):640–648
- Dik VK, Gralnek IM, Segol O, et al. Multicenter, randomized, tandem evaluation of EndoRings colonoscopy—results of the CLEVER study. *Endoscopy* 2015;47(12):1151–1158
- Hassan C, Senore C, Manes G, et al. Diagnostic yield and miss rate of EndoRings in an organized colorectal cancer screening program: the SMART (Study Methodology for ADR-Related Technology) trial. *Gastrointest Endosc* 2019;89(03):583–590.e1
- Triantafyllou K, Polymeros D, Apostolopoulos P, et al. Endocuff-assisted colonoscopy is associated with a lower adenoma miss rate: a multicenter randomized tandem study. *Endoscopy* 2017;49(11):1051–1060
- Aziz M, Haghbin H, Gangwani MK, et al. Efficacy of Endocuff Vision compared to first-generation Endocuff in adenoma detection rate and polyp detection rate in high-definition colonoscopy: a systematic review and network meta-analysis. *Endosc Int Open* 2021;9(01):E41–E50
- Patel HK, Chandrasekar VT, Srinivasan S, et al. Second-generation distal attachment cuff improves adenoma detection rate: meta-

- analysis of randomized controlled trials. *Gastrointest Endosc* 2021;93(03):544–553.e7
- 11 Ngu WS, Bevan R, Tsiamoulos ZP, et al. Improved adenoma detection with Endocuff Vision: the ADENOMA randomised controlled trial. *Gut* 2019;68(02):280–288
 - 12 Rees CJ, Brand A, Ngu WS, et al; B-ADENOMA trial group comprises. BowelScope: accuracy of detection using Endocuff Optimisation of Mucosal Abnormalities (the B-ADENOMA Study): a multicentre, randomised controlled flexible sigmoidoscopy trial. *Gut* 2020;69(11):1959–1965
 - 13 Rex DK, Slaven JE, Garcia J, Lahr R, Searight M, Gross SA. Endocuff vision reduces inspection time without decreasing lesion detection: a clinical randomized trial. *Clin Gastroenterol Hepatol* 2020; 18(01):158–162.e1
 - 14 Jacob A, Schafer A, Yong J, et al. Endocuff Vision-assisted colonoscopy: a randomized controlled trial. *ANZ J Surg* 2019;89(05):E174–E178
 - 15 Rameshshanker R, Tsiamoulos Z, Wilson A, et al. Endoscopic cuff-assisted colonoscopy versus cap-assisted colonoscopy in adenoma detection: randomized tandem study-Detection in Tandem Endocuff Cap Trial (DETECT). *Gastrointest Endosc* 2020;91(04): 894–904.e1
 - 16 Marsano J, Johnson S, Yan S, et al. Comparison of colon adenoma detection rates using cap-assisted and Endocuff-assisted colonoscopy: a randomized controlled trial. *Endosc Int Open* 2019;7: E1585–E1591
 - 17 Rex DK, Sagi SV, Kessler WR, et al. A comparison of 2 distal attachment mucosal exposure devices: a noninferiority randomized controlled trial. *Gastrointest Endosc* 2019;90(05):835–840.e1
 - 18 von Figura G, Hasenöhr M, Haller B, et al. Endocuff vision-assisted vs. standard polyp resection in the colorectum (the EVASTA study): a prospective randomized study. *Endoscopy* 2020;52 (01):45–51
 - 19 Karsenti D, Tharsis G, Perrot B, et al. Adenoma detection by Endocuff-assisted versus standard colonoscopy in routine practice: a cluster-randomised crossover trial. *Gut* 2020;69(12): 2159–2164