

Predictive Accuracy of Wideband Absorbance at Ambient and Tympanometric Peak Pressure Conditions in Identifying Children with Surgically Confirmed Otitis Media with Effusion

Venkatesh Aithal^{1,2} Sreedevi Aithal^{1,2} Joseph Kei² Shane Anderson³ David Wright³

¹ Audiology Department, Townsville Hospital and Health Service, Douglas, Queensland, Australia

² Hearing Research Unit for Children, SHRS, University of Queensland, Queensland, St Lucia, Australia

³ Ear, Nose and Throat Department, Townsville Hospital and Health Service, Queensland, Douglas, Australia

Address for correspondence Venkatesh Aithal, Audiology Department, Townsville Hospital and Health Service, Douglas, Queensland, Australia (e-mail: venkatesh.aithal@health.qld.gov.au).

J Am Acad Audiol 2020;31:471–484.

Abstract

Background Wideband absorbance (WBA) measured at ambient pressure (WBA_A) does not directly account for middle ear pressure effects. On the other hand, WBA measured at tympanometric peak pressure (TPP) (WBA_{TPP}) may compensate for the middle ear pressure effects. To date, there are no studies that have compared WBA_A and WBA_{TPP} in ears with surgically confirmed otitis media with effusion (OME).

Purpose The purpose of this study was to compare the predictive accuracy of WBA_A and WBA_{TPP} in ears with OME.

Research Design Prospective cross-sectional study.

Study Sample A total of 60 ears from 38 healthy children (mean age = 6.5 years, SD = 1.84 years) and 60 ears from 38 children (mean age = 5.5 years, SD = 3.3 years) with confirmed OME during myringotomy were included in this study.

Data Collection and Analysis Results were analyzed using descriptive statistics and analysis of variance. The predictive accuracy of WBA_A and WBA_{TPP} was determined using receiver operating characteristics (ROC) analyses.

Results Both WBA_A and WBA_{TPP} were reduced in ears with OME compared with that in healthy ears. The area under the ROC (AROC) curve was 0.92 for WBA_A at 1.5 kHz, whereas that for WBA_{TPP} at 1.25 kHz was 0.91. In comparison, the AROC for 226-Hz tympanometry based on the static acoustic admittance (Y_{tm}) measure was 0.93.

Conclusions Both WBA_A and WBA_{TPP} showed high and similar test performance, but neither test performed significantly better than 226-Hz tympanometry for detection of surgically confirmed OME.

Key words

- ▶ ambient pressure
- ▶ glue ear
- ▶ otitis media with effusion
- ▶ test performance
- ▶ tympanometric peak pressure
- ▶ wideband absorbance

Introduction

Otitis media with effusion (OME) is defined as the presence of fluid in the middle ear without signs or symptoms of acute

ear infection (Stool et al⁵⁰; Shekelle et al⁴⁹). OME in children can lead to reduced hearing sensitivity and deficits in speech and language development (Wallace et al⁵⁶; Friel-Patti and Finitzo¹¹; Roberts and Wallace³⁹). Normal hearing is a

Copyright © 2020 by the American Academy of Audiology. All rights reserved. Thieme Medical Publishers, Inc., 333 Seventh Avenue, New York, NY 10001, USA. Tel: +1(212) 760-0888.

DOI <https://doi.org/10.3766/jaaa.19012>.
ISSN 1050-0545.

prerequisite for normal speech and language development, but a hearing loss of >15 dB HL can be handicapping for children (Northern and Downs³⁴). Presence of OME can cause a conductive hearing loss of varying degrees which can be transient or of long duration. Hearing loss caused by OME can vary from 0- to 50-dB HL averaged across the speech frequencies (Bess⁷; Fria et al¹⁰; Hunter et al²⁰). Because a large portion of conversational speech does not exceed 50-dB SPL, even a minimal conductive loss could compromise a child's ability to understand speech.

Binaural hearing (Hall et al¹⁵; Yonovitz et al⁵⁹; Aithal et al⁵), auditory processing (Keogh et al²⁹; Graydon et al¹²), academic success (Aithal et al⁴), and speech and language development (Winiger et al⁵⁸) have been shown to be compromised in children with long-lasting OME. Numerous studies have reported delays in speech and language development for children with early onset of OME compared with typically developing children (Klausen et al³⁰; Winiger et al⁵⁸). However, studies addressing the long-term effects of OME on language development have reported contradictory findings. For instance, Teele et al⁵² and Shaffer et al⁴⁸ found significant positive correlations between long-standing OME in the first three years of life and articulation and language-related skills. Unsurprisingly, Paradise et al³⁸ found no relationship between early onset of OME and later language comprehension and production abilities.

Because early onset OME has the potential to impact on children's speech and language and education, it is important to regularly review young children with hearing loss to monitor their hearing sensitivity, speech and language development, and academic progress. Nevertheless, measuring hearing status and middle ear function can be challenging in this population as they are not always co-operative for testing.

Tympanometry using a 226-Hz probe tone is the standard test for assessment of middle ear function in children and adults. The sensitivity of tympanometry in identifying OME, when compared with myringotomy, is reported to be 80–90% and specificity from 74% to 100% (Finitzo et al⁹; Nozza et al^{35,36}; Watters et al⁵⁷; Palmu et al³⁷; Takata et al⁵¹; Harris et al¹⁷). Tympanometric width, or sharpness of the tympanogram shape, has been demonstrated to be the best single criterion for detecting OME with a sensitivity of 81% and specificity of 82% (Nozza et al^{35,36}). Nevertheless, the diagnostic use of tympanograms for identification of OME is limited, especially with tympanograms demonstrating negative middle ear pressure (e.g., <-150 daPa). Studies have found that identification of OME based on negative tympanometric peak pressure (TPP) findings do not adequately separate normal ears from ears with OME (Lildholdt³¹; Shanks and Shelton⁴⁷; Nozza et al³⁶).

In the last decade, research has shown that wideband acoustic immittance (WAI) is a sensitive test of middle ear function. Of the various measures of WAI, wideband absorbance (WBA) is gaining popularity for use in research and clinical settings. The additional WAI measures include resonance frequency, equivalent ear canal volume, TPP, admittance magnitude, and phase angle. WBA is defined as the ratio of energy absorbed by the middle ear to incident acoustic energy

supplied by the probe receiver (Ellison et al⁸). Most earlier studies focused on measuring WAI at ambient pressure. WBA at ambient pressure (WBA_A) is shown to be effective in identifying middle ear dysfunction and conductive disorders in infants (Sanford et al⁴³; Hunter et al¹⁹; Aithal et al³; Aithal et al²), children (Keefe and Simmons²⁷; Keefe et al²⁶), and adults (Margolis et al³²; Shahnaz and Bork⁴⁴; Shahnaz et al⁴⁵). In particular, studies have shown WBA_A to be useful in identifying OME in infants and children (Margolis et al³³; Jeng et al²²; Hunter, Tubaug, et al²¹; Beers et al⁶; Ellison et al⁸; Terzi et al⁵³).

Myringotomy is considered as the gold standard to determine the presence or absence of OME. As myringotomy is an invasive procedure, which requires general anesthesia in children, it is not performed on asymptomatic children for ethical considerations. The lack of effusion may be confirmed by pneumatic otoscopy and hence could be used as a reference standard instead of myringotomy (Rosenfeld et al⁴⁰). Ellison et al⁸ investigated the use of WBA_A with 44 children with OME confirmed by myringotomy and 44 children without a history of middle ear disorders based on surgery and normal pneumatic otoscopic findings. They found that WBA_A was reduced in ears with OME compared with ears from the control group. The test performance of WBA_A in identifying OME was high with area under the receiver operating characteristic (AROC) curve of 0.93. Terzi et al⁵³ assessed 34 typically developing children, 44 children diagnosed with OME during myringotomy, and 28 children with OME but no signs of effusion during myringotomy. Terzi et al⁵³ reported that WBA_A was significantly lower in the OME group. In evaluating the test performance of the WBA_A test, they found that WBA in the frequency region 0.375–2 kHz had the highest AROC of 0.984, followed by that at 1 and 1.5 kHz of 0.973 and 0.967, respectively. In another study, Beers et al⁶ compared WBA_A in 78 children who passed a battery of tests with that of 25 children with OME confirmed by video otomicroscopy and pneumatic otoscopy. They reported that WBA_A >0.8 kHz had high test performance in distinguishing normal middle ear status from OME. They found that WBA_A at 1.25 kHz had the highest AROC of 0.97.

Surprisingly, there is limited research regarding comparison of test performance of WBA with conventional 226-Hz tympanometry. Studies have suggested that WBA_A is significantly better than 226-Hz tympanometry in distinguishing ears with OME from normal middle ears (Beers et al⁶; Terzi et al⁵³) and predicting conductive hearing loss in young children due to OME (Keefe et al²⁶). Keefe et al²⁶ noted that both WBA_A and tympanometric WBA showed better test performance compared with 226-Hz tympanometry in children.

The aforementioned studies have measured WBA_A. WBA can also be measured under tympanometric pressurized conditions, known as wideband tympanometry (WBT). WBT provides additional information of middle ear function compared with WBA_A measurements, by measuring absorbance at TPP (WBA_{TPP}). Earlier studies have suggested that WBA_{TPP} may be more sensitive to middle ear disorders in children and adults (Margolis et al³²; Keefe and Simmons²⁷; Sanford and Feeney⁴²). More recently, Keefe et al²³ evaluated normal and surgically confirmed otosclerotic ears and using

a multivariate predictor with three reflectance variables and reported that tympanometric reflectance was more accurate than ambient reflectance (AROC 0.95 versus AROC 0.88) in classifying ears as normal or otosclerotic ears. However, other studies have shown similar test performance for WBA_A and WBA_{TPP} for identifying middle ear dysfunction and conductive hearing loss (Sanford et al⁴³; Keefe et al²⁶).

Margolis et al³² suggested that it may be potentially advantageous to assess middle ear function using both WBA_A and WBA_{TPP} procedure. The researchers reported a single case study of a ten-year-old child with a conductive loss of 35-dB HL and TPP of -250 daPa. They found the absorbance to be abnormal even when the ear canal was pressurized to match the TPP and suggested that pathologic middle ear changes might have occurred in addition to the presence of negative pressure in the middle ear (Margolis et al³²).

By measuring absorbance at TPP, WBT provides additional information of middle ear function compared with WBA_A measurements. More importantly, WBT produces an optimal WBA_{TPP} response by compensating for the effect of the difference in pressure between the ear canal and the middle ear. WBT generates a three-dimensional plot of absorbance as function of both ear canal pressure and frequency. From this plot, WBA at any applied pressure, including TPP, can be derived. WBA_A evaluates middle ear function without adjusting for middle ear pressure effects. But WBA_{TPP} evaluates middle ear function after compensating for the difference in pressure between the outer ear and the middle ear. Hence, measuring WBA at TPP will reduce the middle ear pressure effects and measure changes in absorbance due to the middle ear pathology per se.

Although many researchers have studied WBA_A in ears with OME based on otoscopy and audiological findings, surgical confirmation of OME is important and significant as otoscopic measures are often subjective and less reliable. To date, there are only two studies that have investigated WBA_A in ears with surgically confirmed OME (Ellison et al⁸; Terzi et al⁵³). However, neither of these studies have studied WBA_{TPP} . The purpose of the present study was to compare the predictive accuracy of WBA_A and WBA_{TPP} in ears with OME confirmed by myringotomy.

Materials and Methods

Participants

The study was approved by Townsville Hospital and Health Service Ethics Board. Written consent was obtained from parents or carers. The participants were divided into two groups.

Control Group

The control group consisted of 60 healthy ears (35 right and 25 left) from 38 children (25 males and 13 females) who presented to the audiology clinic with no history of ear or hearing difficulties. Mean age at the time of testing was 6.5 years (standard deviation [SD] = 1.84, range 4.11–11.4 years). Inclusion criteria for the control group were as follows: (a) no significant history of middle ear infection at

the time of testing, (b) normal otoscopic findings, (c) normal tympanogram with peak Y_{tm} between 0.3 and 1.4 mmhos and TPP between -100 and 100 daPa, (d) air conduction (AC) thresholds <20 -dB HL between 0.25 and 8 kHz, (e) air-bone gap of <15 dB at frequencies between 0.25 and 4 kHz, and (f) a pass in transient evoked otoacoustic emissions (TEOAEs) as determined by signal to noise ratio of ≥ 3 dB at 2, 3, and 4 kHz (Kei et al²⁸).

OME Group

Children with OME as determined by an ear nose and throat (ENT) specialist and who were scheduled for myringotomy with or without grommet insertion were enrolled in the OME group. Initial diagnosis of OME was made based on otomicroscopy by the ENT specialist. Subject data were only included in the OME group if the ENT specialist confirmed the presence of effusion during myringotomy. This group consisted of 60 ears (30 right and 30 left) from 38 children (25 males and 13 females). The ENT specialist subjectively rated middle ear fluid as thick or thin during surgery. Thick fluid was noted in 37 ears and thin fluid in 23 ears. Mean age at the time of diagnosis was 5.5 years (SD = 3.3 years, range 1.1–14.3 years). There was no significant difference between the mean age of two groups [$t_{(74)} = -1.64, p = 0.11$].

Test Procedure

All testing was performed by a clinical audiologist in a sound-treated room with ambient noise <35 -dB A. Testing was scheduled at least one hour before the surgery. Although both ears were tested, only the ear with surgically confirmed OME was included in the study. Tympanometry, TEOAEs, pure-tone audiometry, WBA_A , and WBA_{TPP} were performed in no particular order.

Tympanometry

Tympanometry was performed using a GSI Tymp Star 2 middle ear analyzer (Grason-Stadler; Eden Prairie, MN). Tympanograms were obtained by presenting a 226-Hz probe tone at 85-dB SPL to the ear while the ear canal pressure was varied from $+200$ to -400 daPa. Quantitative tympanometric measures of peak compensated static acoustic admittance measured between the peak and 200 daPa (Y_{tm} in mmho) and TPP in daPa were used to classify tympanograms as normal, flat, or negative middle ear pressure. Tympanograms with static admittance between 0.3 and 1.4 mmho and middle ear pressure of between -100 and 100 daPa were classified as normal. Tympanograms with static admittance <0.3 mmho with no identifiable peak were classified as flat tympanograms, and tympanograms with middle ear pressure <-100 daPa as negative middle ear pressure (Nozza et al^{35,36}; Valente et al⁵⁴).

TEOAEs Test

A Biologic Scout Version.3.45 (Natus; San Carlos, CA) was used to measure TEOAEs. The signal consisted of wideband clicks of 80- μ s duration, at a target amplitude of 80-dB peak-equivalent sound pressure level. The pass criteria included reproducibility of $\geq 70\%$ and a difference between the

amplitude of the emission and the associated noise floor of ≥ 3 dB at 2, 3, and 4 kHz (Kei et al²⁸; Vander Werff et al⁵⁵).

Audiometry

AC and bone conduction (BC) audiometry were performed using an Interacoustic AC 40 audiometer (Interacoustics; Assens, Denmark). Thresholds were determined using the Hughson-Westlake Method. Conditioned play audiometry was used for children aged between 2.5 and 5 years. AC thresholds were measured at 0.25, 0.5, 1, 2, 4, and 8 kHz and BC thresholds were measured at 0.25, 0.5, 1, 2, and 4 kHz. Air-bone gap data were obtained at all BC test frequencies.

Visual reinforcement audiometry was performed for children younger than 2.5 years using an Interacoustic AC 40 audiometer with a free field setup. Visual reinforcement audiometry thresholds were determined for warble tones at 0.5, 1, 2, and 4 kHz presented through a loudspeaker kept at 1-m distance at an angle of 45° from the child's ears.

Wideband Absorbance Measurements and Analysis

Both WBA_A and WBA_{TPP} were measured using a prototype system developed by Interacoustics (Keefe et al²⁵; Sanford et al⁴³; Aithal et al³). The Reflwin computerized system consisted of a Windows-based computer, a 24-bit resolution sound card, a pressure pump and controller system containing an acoustic immittance instrument (AT235), and custom software (version 3.2.1) (Interacoustics, Assens, Denmark) for stimulus generation and data acquisition. Calibration was performed every day before data collection (Keefe and Simmons²⁷; Sanford and Feeney⁴²). Calibration was performed at ambient pressure to determine the source reflectance and incident sound pressure associated with the probe and its transducers based on acoustic measurements in four rigid-walled cylindrical calibration tubes that were open at one end and closed at the other with a steel rod. The infant calibration tubes had lengths of 232.11 and 53.19 mm, each with a diameter of 4.8 mm (small-tube) and the adult calibration tubes had lengths of 290.50 and 81 mm, each with a diameter of 7.9 mm (large-tube). A root mean squared reflectance error of <0.009 was required for successful calibration and any calibration that did not meet the criteria was repeated after the probe reinsertion. Reflectance is the ratio of reflected energy at the probe termination in the ear canal to incident acoustic energy supplied by the probe receiver (Ellison et al⁸). Absorbance is defined as 1–reflectance. Responses in the age group equal to or older than 0.5 years were analyzed with respect to large-tube calibration and newborns through 0.4 years were analyzed with respect to small-tube calibration. However, in the present study, only adult calibration values were used as the youngest child tested was only 1.1 year old.

Measurements were obtained by recording acoustic response to clicks presented at 55 dB SPL at a rate of one click per 46 msec. Responses from a total of 32 clicks were averaged for each measurement and reflectance was calculated for each response. The response consisted of 16 data points at 1/3 octave frequencies from 226 to 8000 Hz. WBA_A was always measured before WBA_{TPP} . WBT testing was performed using

Reflwin software in combination with the modified acoustic immittance instrument (AT 235). A slow pump speed of 75 daPa/sec was used and the pressure was swept from +200 to –300 daPa, respectively. Visual inspection of the absorbance curve was performed to determine adequate probe fit. Absorbance more than 0.29 in the low frequency band (0.25–0.5 kHz) was indicative of a probe leak (Groot et al¹⁴). When probe leakage was suspected, the probe was reinserted, and the test was repeated.

Data were exported to an Excel spreadsheet using a MATLAB software (R2014b) (The MathWorks Inc, Natick, MA). The data were then transferred into the IBM SPSS (version 23) (IBM Corporation, Armonk, NY) for further analysis. Mean WBA_A and WBA_{TPP} were determined for 16 one-third octave frequencies from 0.25 to 8 kHz and were also obtained for frequencies between 0.3 and 2 kHz, 1 and 2 kHz, and 2 and 8 kHz. WBA_A was measured at ambient pressure in the ear canal whereas WBA_{TPP} was measured at TPP. TPP was measured by calculating the pressure at which the maximum of low-frequency averaged absorbance (0.376–2 kHz) occurred. It was automatically calculated by the program. For tympanograms with no peaks, the program identified the maximum-averaged absorbance point and measured the TPP. In this case, the TPP does not necessarily indicate the difference in pressure between the ear canal and middle ear cavity.

Statistical analysis was performed using the IBM SPSS software version 23. A mixed model analysis of variance (ANOVA) was used to analyze data for ears with and without OME. The Greenhouse and Geisser¹³ (G-G) approach was used to compensate for the violation of compound symmetry and sphericity. Data were analyzed using ear status (control versus OME) as between group factor and frequencies as within group factor. Post hoc analyses were performed using multiple pair wise comparison tests with Bonferroni adjustments to determine the frequencies at which significant differences existed between control and OME groups. *p* value of <0.05 was considered statistically significant for all analyses.

Measures of Test Performance

The test performance of WBA_A and WBA_{TPP} to detect OME was determined using ROC analyses. AROC was determined for each of the 16 one-third octave frequencies as well as 0.3–2, 1–2, and 2–8-kHz frequency bands for WBA_A and WBA_{TPP} using SPSS software (version 23).

Results

There was no significant difference in age between the two groups of participants [$t_{(74)} = -1.64, p = 0.11$] (► **Table 1**). An ANOVA was fitted to the WBA_A and WBA_{TPP} data from the control and OME groups to test the significance of difference between right and left ears, and male and females, and their interactions. To analyze the ears and gender, only one ear was selected for the study and in case of children passing both ears, only one ear was selected at random. This was performed to avoid the potential influence of pooling the data across ear for analysis. This resulted 38 ears (24 right and 14 left) for WBA_A and 21 ears (12 right and 9 left) for WBA_{TPP} in

Table 1 Participant Details

	Control Group	OME Group
No. children	38	38
Male	25	25
Female	13	13
Total no. of ears	60	60
Right ear	35	30
Left ear	25	30
Age (years)		
Mean	6.5	5.5
SD	1.84	3.3
Range	4.11–11.4	1.1–14.3

control group. Similarly, 38 ears (22 right and 16 left) were selected for WBA_A and 32 ears (19 right and 13 left) for WBA_{TPP} in the OME group. Less ears were selected for WBA_{TPP} condition as data were not available for all children for the TPP conditions.

For the control group, results of an ANOVA fitted to the data obtained from WBA_A showed no significant difference between ears, $F_{(1, 34)} = 1.01, p > 0.05$; gender, $F_{(1, 34)} = 0.06, p > 0.05$ and ear X gender interaction, $F_{(1, 34)} = 0.06, p > 0.05$. Likewise, no significant difference between ears, $F_{(1, 17)} = 2.47, p > 0.05$; gender, $F_{(1, 17)} = 0.04, p > 0.05$; and ear X gender interaction, $F_{(1, 17)} = 0.01, p > 0.05$ were observed for the WBA_{TPP} measure.

For the OME group, results of an ANOVA fitted to the data obtained from WBA_A showed no significant difference between ears, $F_{(1, 34)} = 1.24, p > 0.05$; gender, $F_{(1, 34)} = 0.17, p > 0.05$; and ear X gender interaction, $F_{(1, 34)} = 1.15, p > 0.05$. Likewise, no significant difference between ear, $F_{(1, 28)} = 0.73, p > 0.05$; gender, $F_{(1, 28)} = 1.06, p > 0.05$; and ear X gender interaction, $F_{(1, 28)} = 0.05, p > 0.05$ were observed for the WBA_{TPP} measure. Subsequently, ears were pooled for both groups for further analysis.

The tympanometric data were analyzed based on quantitative analyses. All the 60 ears from 38 children in the control group had normal tympanogram with Y_{tm} between 0.3 and 1.4 mmhos (mean = 0.57 mmho, SD = 0.23 mmho, range = 0.3–1.1 mmho) and TPP of within 6100 daPa (mean = -10 daPa, SD = 35.58 daPa, range = -100 to 30). In the OME group, a total of 52 ears had flat tympanograms and six ears had negative middle ear pressure with a mean TPP of -200 daPa (SD = 95 daPa, range = -105 to -335 daPa) and normal Y_{tm} . Two ears had normal tympanograms with a mean TPP of -17 daPa (range = -45 to 10 daPa) and normal Y_{tm} .

Complete TEOAE data sets were available for the control group but not for the OME group. All 60 ears of children in the control group passed the TEOAE test. In the OME group, four ears passed and 36 ears failed the TEOAE test. TEOAE data were not available for 20 ears mainly because of lack of cooperation from the child and insufficient time as tests were performed one hour before the surgery.

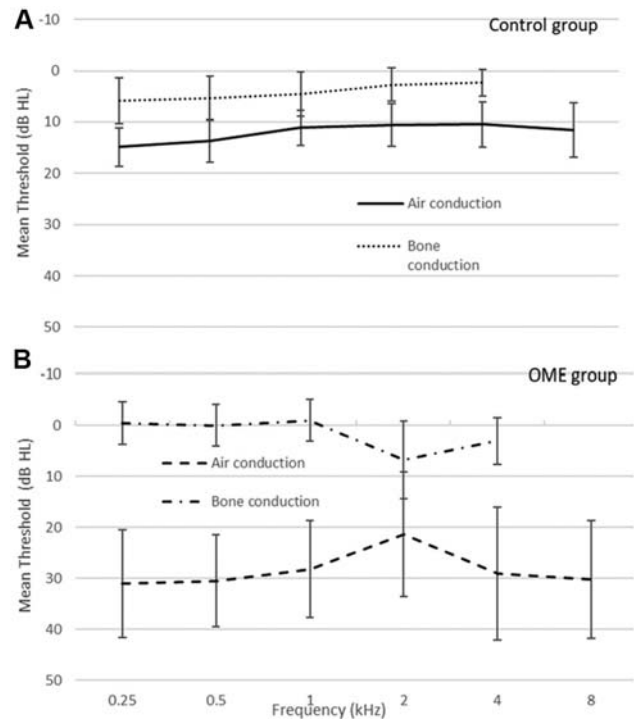


Fig. 1 Mean AC and BC thresholds of participants in (A) control and (B) OME group. Error bar denotes ± 1 SD.

Initially, 93 ears from 58 children were suspected to have OME based on otoscopic and audiometric findings. Of these, 33 ears from 20 children were found not to have fluid during surgery. Effusion was noted in 60 ears from 38 children during surgery and only results from ears with confirmed OME were used for further analysis and to test the predictive accuracy of WBA.

► **Figure 1** shows the mean AC and BC thresholds of ears in the control and OME group. AC and BC thresholds were available for all 60 ears of 38 children in the control group and 30 ears of 19 children in the OME group. The OME group demonstrated a mild conductive hearing loss throughout the frequency range with better AC thresholds, but worse BC thresholds at 2 kHz than that at other frequencies.

► **Figure 2(A)** illustrates mean WBA_A and shaded area (interquartile range [IQR], range between 25th and 75th percentiles) from 0.25 to 8 kHz for the control and OME groups. Error bar shows mean ± 1 standard error of mean (SEM). Mean WBA_A for both groups showed a single-peaked pattern at 3 kHz. Mean WBA_A of the control group increased gradually from 0.09 at 0.25 kHz to reach a maximum of 0.86 at 3 kHz, and then decreased rapidly with frequency to 0.14 at 8 kHz. In comparison, mean WBA_A of the OME group varied between 0.08 and 0.28 from 0.25 to 1.5 kHz, increased gradually until it reached a maximum of 0.42 at 3 kHz, and then decreased rapidly with frequency to 0.17 at 8 kHz. Mean WBA_A of the OME group was below the 25th percentile of mean WBA_A of the control group at all frequencies between 0.4 and 6 kHz. In comparison, mean WBA_A of the control group was above the 75th percentile of the OME group at all frequencies.

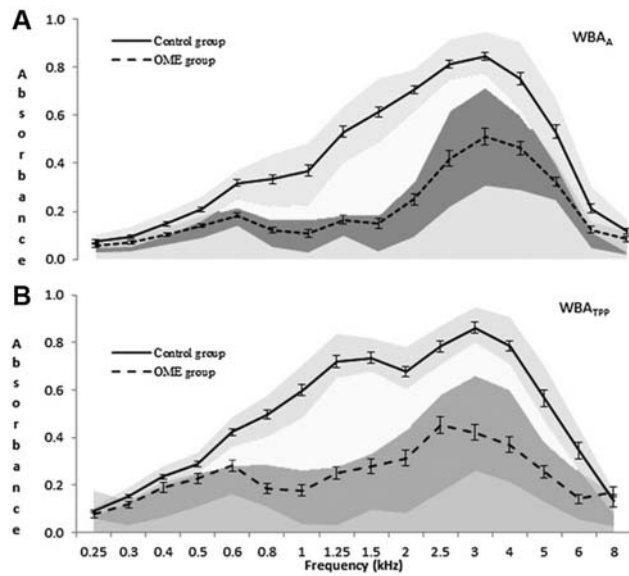


Fig. 2 (A) Mean WBA_A and IQR from 0.25 to 8 kHz for the control and OME group. (B) Mean WBA_{TPP} and IQR from 0.25 to 8 kHz for the control and OME group. Vertical bars denote mean ± 1 SEM. Shaded areas denote IQR (control group—light gray shading; OME group—dark gray shading).

An ANOVA was performed with WBA_A as the dependent variable and ear condition (control versus OME group) and frequency as independent variables. The results showed a significant main effect for ear condition [$F_{(1, 118)} = 293.01$,

$p < 0.001$, partial eta square = 0.71, observed power = 1]. The main effect of frequency [$F_{(4, 468)} = 280.68$, $p < 0.001$, partial eta square = 0.70, observed power = 1] and interaction between ear condition and frequency [$F_{(4, 468)} = 45.15$, $p < 0.001$, partial eta square = 0.28, observed power = 1] were also significant.

A series of t-tests applied to the WBA_A data showed that mean WBA_A of the OME group was significantly lower than that of the control group at frequencies between 0.25 and 6 kHz and frequency bands of 0.3–2, 1–2, and 2–8 kHz (**Table 2**).

The results of an ANOVA with WBA_{TPP} as the dependent variable showed a significant main effect for ear condition [$F_{(1, 55)} = 77.43$, $p < 0.001$, partial eta square = 0.59, observed power = 1]. The main effect of frequency [$F_{(4, 259)} = 8.48$, $p < 0.001$, partial eta square = 0.59, observed power = 1] and interaction between ear conditions and frequency [$F_{(4, 259)} = 20.95$, $p < 0.001$, partial eta square = 0.28, observed power = 1] were also significant.

Figure 2(B) illustrates the mean WBA_{TPP} and IQR from 0.25 to 8 kHz for the control and OME groups. Mean WBA_{TPP} for the control group showed two large peaks with the first peak occurring at 1.25–1.5 kHz and the second peak at 3 kHz. Mean WBA_{TPP} was reduced < 1.25 and > 3 kHz. In comparison, mean WBA_{TPP} of the OME group showed a large peak occurring at 2.5 kHz. Mean WBA_{TPP} of OME group was lower than that of the 25th percentile of the control group at all frequencies between 0.4 and 6 kHz. On the other hand, mean

Table 2 Mean, SEM, Significance of Difference and Magnitude of Effect in WBA_A between the Control and Otitis Media with Effusion (OME) Group

Frequency (kHz)	Control Group, n = 60 Ears Mean \pm SEM	OME Group, n = 60 Ears Mean \pm SEM	t-Value	Eta Square	Observed Power
0.25	0.08 \pm 0.01	0.06 \pm 0.01	2.16*	0.04	0.57
0.3	0.09 \pm 0.01	0.07 \pm 0.01	2.28*	0.04	0.62
0.4	0.15 \pm 0.01	0.10 \pm 0.01	3.77*	0.11	0.96
0.5	0.21 \pm 0.01	0.14 \pm 0.01	5.02*	0.18	0.99
0.6	0.32 \pm 0.01	0.18 \pm 0.01	8.13*	0.36	1.00
0.8	0.33 \pm 0.02	0.12 \pm 0.02	8.81*	0.40	1.00
1	0.37 \pm 0.02	0.11 \pm 0.02	8.91*	0.40	1.00
1.25	0.53 \pm 0.02	0.17 \pm 0.02	11.87*	0.54	1.00
1.5	0.61 \pm 0.02	0.15 \pm 0.02	15.24*	0.66	1.00
2	0.70 \pm 0.02	0.25 \pm 0.02	16.07*	0.69	1.00
2.5	0.81 \pm 0.02	0.42 \pm 0.02	11.04*	0.51	1.00
3	0.85 \pm 0.02	0.51 \pm 0.02	8.52*	0.38	1.00
4	0.75 \pm 0.03	0.46 \pm 0.03	7.77*	0.34	1.00
5	0.53 \pm 0.03	0.32 \pm 0.03	6.04*	0.24	1.00
6	0.21 \pm 0.02	0.12 \pm 0.02	3.96*	0.12	0.98
8	0.12 \pm 0.01	0.09 \pm 0.01	1.89	0.03	0.47
0.3–2	0.37 \pm 0.01	0.14 \pm 0.01	13.56*	0.61	1.00
1–2	0.55 \pm 0.02	0.17 \pm 0.02	15.28*	0.66	1.00
2–8	0.57 \pm 0.01	0.31 \pm 0.01	13.81*	0.62	1.00

*Significant difference with $p < 0.05$.

Table 3 Mean, SEM, Significance of Difference and Magnitude of Effect in WBA_{TPP} between the Control and OME Group

Frequency (kHz)	Control Group, n = 60 Ears Mean ± SEM	OME Group, n = 60 Ears Mean ± SEM	t-Value	Eta Square	Observed Power
0.25	0.09 ± 0.01	0.08 ± 0.02	21.98	0.07	0.49
0.3	0.15 ± 0.01	0.12 ± 0.02	1.57	0.05	0.34
0.4	0.24 ± 0.01	0.19 ± 0.02	1.61	0.05	0.35
0.5	0.29 ± 0.01	0.23 ± 0.02	1.53	0.04	0.32
0.6	0.42 ± 0.01	0.28 ± 0.02	3.22*	0.17	0.89
0.8	0.49 ± 0.02	0.18 ± 0.02	5.05*	0.33	1.00
1	0.60 ± 0.02	0.18 ± 0.02	7.56*	0.53	1.00
1.25	0.72 ± 0.03	0.25 ± 0.03	9.28*	0.63	1.00
1.5	0.74 ± 0.02	0.28 ± 0.03	7.88*	0.55	1.00
2	0.68 ± 0.02	0.31 ± 0.03	6.85*	0.48	1.00
2.5	0.78 ± 0.02	0.45 ± 0.04	6.52*	0.45	1.00
3	0.86 ± 0.02	0.42 ± 0.03	6.88*	0.48	1.00
4	0.78 ± 0.03	0.37 ± 0.03	5.62*	0.38	1.00
5	0.56 ± 0.03	0.26 ± 0.03	4.97*	0.33	1.00
6	0.35 ± 0.02	0.14 ± 0.02	4.02*	0.24	0.98
8	0.14 ± 0.03	0.17 ± 0.02	0.28	0.00	0.06
0.3–2	0.62 ± 0.02	0.29 ± 0.02	6.80*	0.48	1.00
1–2	0.68 ± 0.02	0.23 ± 0.03	8.91*	0.61	1.00
2–8	0.60 ± 0.02	0.30 ± 0.02	8.12*	0.56	1.00

*Significant difference with $p < 0.05$.

WBA_{TPP} of the control group was above the 75th percentile of the OME group at all frequencies except 8 kHz.

Mean WBA_{TPP} of the OME group was significantly lower than that of the control group at frequencies between 0.6 and 6 kHz and frequency bands of 0.3–2, 1–2, and 2–8 kHz as indicated by the t-test results (see ►Table 3).

►Figure 3 shows the comparison of mean absorbance at WBA_A and WBA_{TPP} for the control and OME groups. Error bar shows mean ± 1 SEM. An ANOVA was applied to assess the difference in absorbance across the two WBA measures for each group. The results showed a significant difference between the two measures, with WBA_{TPP} showing significantly higher absorbance between 0.3 and 1.5 kHz, and 6 kHz for the control group and between 0.25 and 1.5 kHz, and 6 kHz for the OME group.

►Table 4 summarizes the AROC, 95% confidence intervals (CIs), cutoff value, sensitivity, and specificity of WBA_A and WBA_{TPP} for each of the one-third octave frequency between 0.25 and 8 kHz and frequency bands of 0.3–2, 1–2, and 2–8 kHz. The diagnostic accuracy of WBA_A was higher than 0.7 in the frequency between 0.6 and 4 kHz and frequency bands of 0.3–2, 1–2, and 2–8 kHz. The AROC was highest at 1.5 kHz (0.92) followed by 1.25 kHz (0.90). The sensitivity of WBA_A reached the highest values of 0.92 and 0.88 at 1.5 and 1.25 kHz, respectively. In comparison, the specificity of WBA_A remained high across the entire frequency range.

The diagnostic accuracy of WBA_{TPP} was higher than 0.7 in the frequency between 0.3 and 5 kHz and frequency bands of

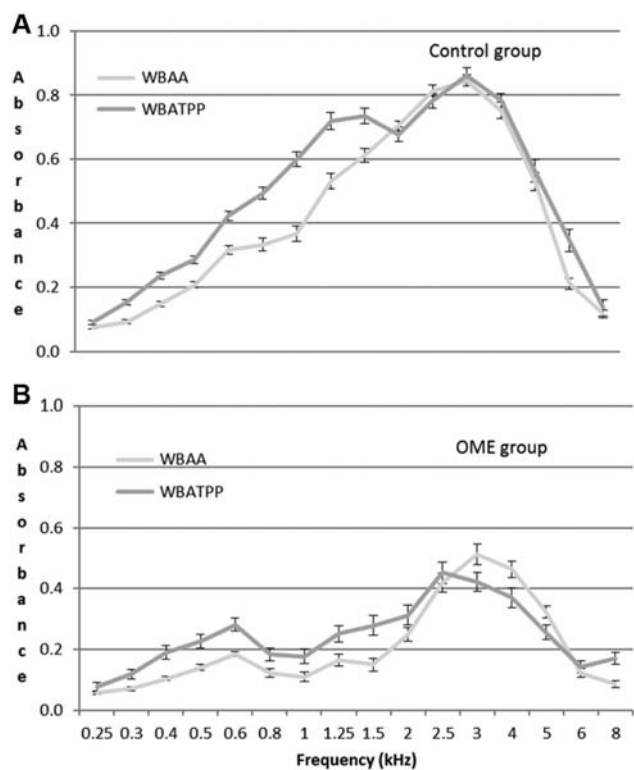


Fig. 3 Comparison of mean WBA_A and WBA_{TPP} conditions for (A) control and (B) OME group. Error bar denotes ±1 SEM. Significant difference with $p < 0.05$ noted at 0.3–1.5 and 6 kHz for control group and 0.25–1.5 and 6 kHz for OME group.

Table 4 The Area Under the Receiver Operating Curve (AROC) and Corresponding CIs, Sensitivity, and Specificity for WBA_A and WBA_{TPP}

Frequency (kHz)	WBA _A					WBA _{TPP}				
	AROC	95% CI	Cutoff WBA _A	Sensitivity	Specificity	AROC	95% CI	Cutoff WBA _{TPP}	Sensitivity	Specificity
0.25	0.45	0.35–0.55	0.01	0.00	0.90	0.58	0.45–0.70	0.05	0.21	0.94
0.30	0.49	0.39–0.60	0.02	0.07	0.92	0.79*	0.69–0.89	0.10	0.64	0.94
0.40	0.56	0.46–0.66	0.06	0.18	0.93	0.79*	0.70–0.89	0.17	0.66	0.94
0.50	0.64	0.54–0.74	0.10	0.35	0.93	0.74*	0.64–0.85	0.20	0.55	0.94
0.60	0.71*	0.61–0.80	0.19	0.50	0.92	0.86*	0.78–0.94	0.32	0.79	0.94
0.80	0.79*	0.71–0.88	0.15	0.67	0.92	0.90*	0.82–0.97	0.33	0.82	0.97
1.00	0.80*	0.72–0.88	0.11	0.68	0.92	0.90*	0.82–0.97	0.36	0.86	0.94
1.25	0.90*	0.84–0.96	0.28	0.88	0.92	0.91*	0.83–0.98	0.54	0.88	0.94
1.50	0.92*	0.86–0.97	0.39	0.92	0.92	0.82*	0.73–0.91	0.53	0.73	0.90
2.00	0.87*	0.80–0.94	0.57	0.73	1.00	0.84*	0.76–0.92	0.50	0.75	0.94
2.50	0.85*	0.78–0.92	0.63	0.78	0.92	0.81*	0.71–0.90	0.60	0.71	0.90
3.00	0.79*	0.71–0.88	0.68	0.72	0.88	0.78*	0.68–0.88	0.61	0.66	0.90
4.00	0.72*	0.62–0.81	0.49	0.53	0.90	0.78*	0.68–0.88	0.55	0.66	0.90
5.00	0.55	0.45–0.65	0.23	0.18	0.92	0.75*	0.65–0.86	0.27	0.57	0.94
6.00	0.58	0.48–0.69	0.05	0.25	0.92	0.66*	0.55–0.78	0.15	0.39	0.94
8.00	0.52	0.41–0.62	0.00	0.03	1.00	0.62	0.50–0.74	0.02	0.34	0.90
0.3–2	0.91*	0.85–0.97	0.24	0.95	0.87	0.86*	0.77–0.94	0.48	0.82	0.92
1–2	0.92*	0.86–0.97	0.38	0.92	0.92	0.88*	0.81–0.96	0.51	0.86	0.90
2–8	0.90*	0.84–0.96	0.44	0.90	0.90	0.88*	0.81–0.96	0.44	0.83	0.93

*Significant difference with $p < 0.05$.

Table 5 Summary of AROC, SEM, and 95% CI for WBA_A, WBA_{TPP}, and 226-Hz Tympanogram (Y_{tm})

	AROC	SEM	95% CI
WBA _A (1.5 kHz)	0.92	0.03	0.86–0.97
WBA _{TPP} (1.2 kHz)	0.91	0.04	0.83–0.98
Y _{tm} (226 Hz)	0.93	0.03	0.88–0.99

0.3–2, 1–2, and 2–8 kHz. The AROC was highest at 1.25 kHz (0.91), followed by 1 and 0.8 kHz (0.90). The sensitivity of WBA_{TPP} reached the highest values of 0.88 and 0.86 at 1.25 and 1 kHz, respectively, whereas the specificity of WBA_{TPP} remained high across the entire frequency range. Statistical significance of the difference in AROC between WBA_A and WBA_{TPP} was determined as suggested by Hanley and McNeil.¹⁶ AROC for WBA_{TPP} was significantly higher than WBA_A at 0.3, 0.4, 0.6, and 5 kHz.

► **Table 5** shows a summary of AROC and corresponding SEM and 95% CI for WBA_A at 1.5-kHz and WBA_{TPP} at 1.2-kHz and 226-Hz Y_{tm} tympanogram. These frequencies were selected because of the optimal performance of WBA at these frequencies. Comparison of AROC among these measures revealed no significant differences among the WBA_A, WBA_{TPP}, and 226-Hz tympanometry.

► **Figure 4** shows a comparison of the mean WBA_A and WBA_{TPP} for the control group with that of the three tympano-

gram types of the OME group. Mean WBA_A of the control group showed a single peak at 3 kHz, whereas mean WBA_{TPP} showed two prominent peaks at 1.5 and 3.5 kHz. For ears with OME with normal tympanogram, both mean WBA_A and WBA_{TPP} showed a single peak. For ears with OME with flat tympanograms, both mean WBA_A and WBA_{TPP} showed the lowest absorbance. For ears with OME with negative middle ear pressure, both WBA_A and WBA_{TPP} showed absorbance in between OME with normal and flat tympanograms.

► **Figure 5** shows a comparison of mean WBA_A for both the control and OME group of the present study with that obtained by Keefe et al.²⁶ and Terzi et al.⁵³ The results of the present study resembled closely with those of the study by Keefe et al.²⁶ Terzi et al.⁵³ showed improved absorbance for their control group ~1–2 kHz and OME group ~1.5–3 kHz.

Subjective rating of the OME fluid as thick or thin by operating ENT surgeon was analyzed in this study. ► **Figure 6** compares WBA_A and WBA_{TPP} for the OME group with thick and thin fluid with that of the control group. Mean WBA_A obtained for both thick and thin fluid conditions were similar. However, mean WBA_{TPP} obtained for the thin fluid was higher than that for thick fluid across 0.25–8 kHz.

Discussion

The results of the study showed no significant ear, gender, or gender by ear interaction effects on WBA_A and WBA_{TPP}. These

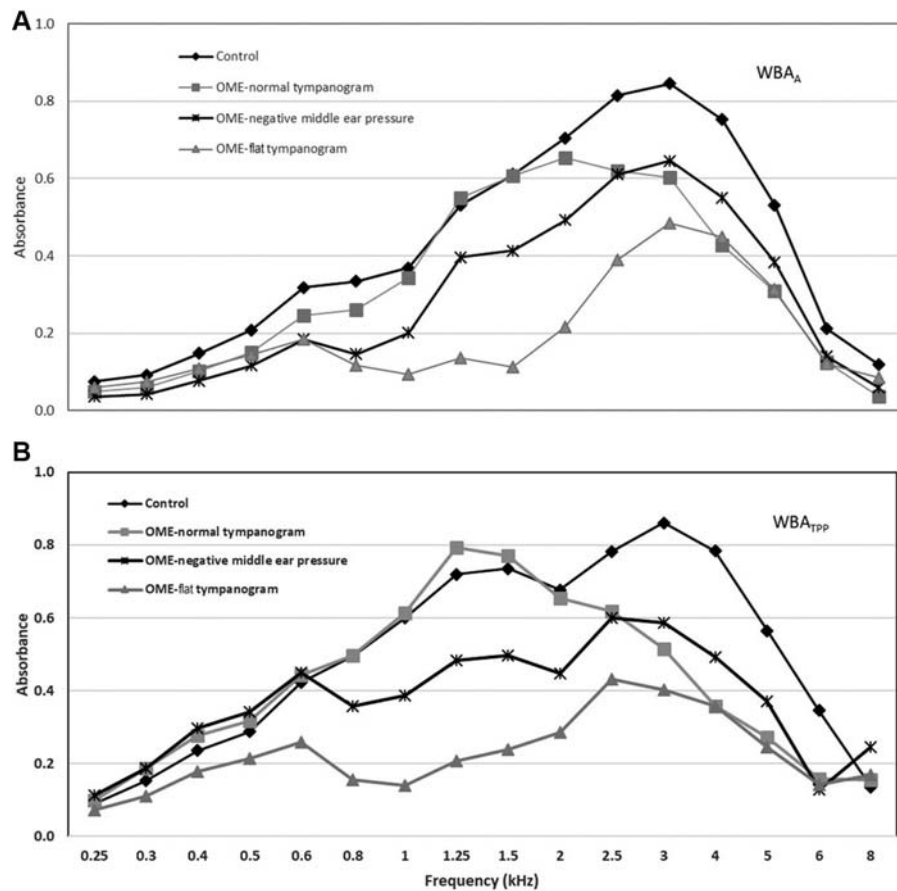


Fig. 4 Comparison of (A) WBA_A and (B) WBA_{TPP} for control group and OME group with different types of tympanograms.

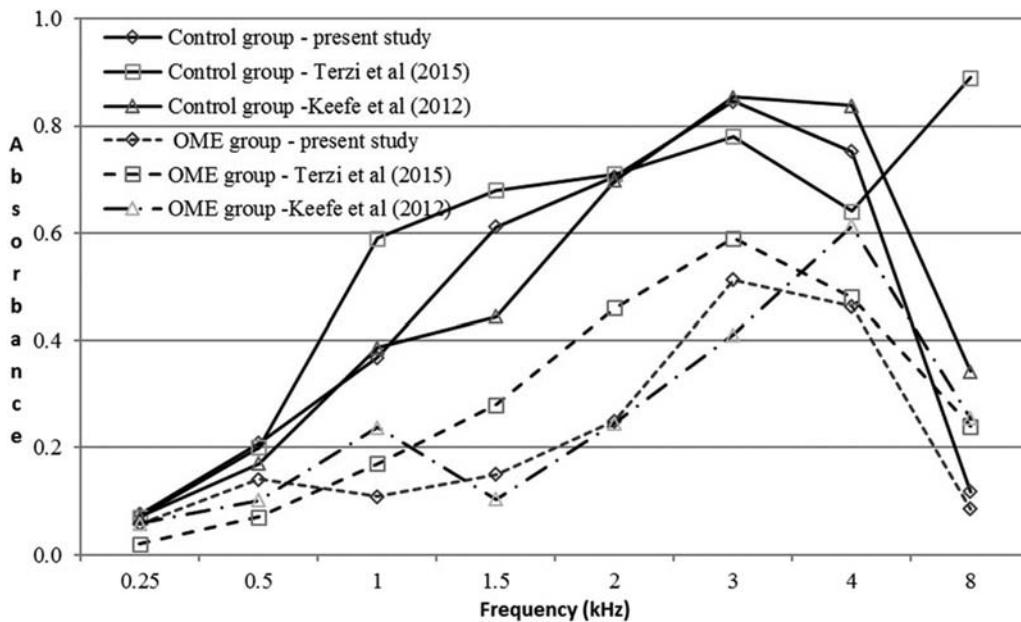


Fig. 5 Comparison of mean WBA_A with control and OME group of the present study with WBA_A of the studies by Keefe et al²⁶ and Terzi et al.⁵³

findings are consistent with the previous studies (Hunter, Bagger-Sjback, et al¹⁸; Beers et al⁶), which reported no significant differences in WBA_A across ears and genders. On the other hand, the effect of gender on WBA_A is inconclusive. For example, Shahnaz et al⁴⁶ reported that

WBA_A varies differently between females and males across frequencies. The males had lower absorbance at 4 and 5 kHz than females. Although the source of these ear and gender differences is not known, it may be partly due to the methodological differences, including age range of

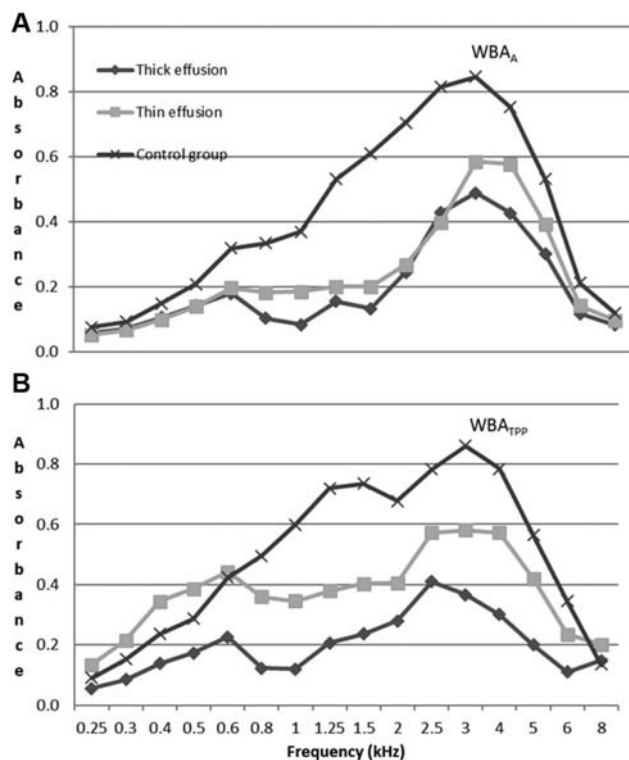


Fig. 6 Comparison of (A) WBA_A and (B) WBA_{TPP} for control and OME group with thick and thin effusion as determined by ENT surgeon during surgery.

participants, equipment, calibration, and selection criteria used in the respective studies.

In the present study, results showed a significant group effect for ear conditions (control versus OME group) for both WBA_A and WBA_{TPP} . This study also noted a significant main effect for frequency and frequency by ear conditions for both WBA_A and WBA_{TPP} tests, suggesting that the absorbance pattern across frequency was different for each group. Mean WBA_A of the control group increased gradually from 0.25 kHz to reach a maximum at 3 kHz. In comparison, mean WBA_A of the OME group was relatively stable with only 10% variation and increasing gradually to reach a maximum at 3 kHz. Mean WBA_A of the OME group was lower than the 25th percentile of WBA_A of control group at all frequencies between 0.4 and 6 kHz. In comparison, mean WBA_A of the control group was above the 75th percentile of the OME group at all frequencies (→ **Figure 2A**).

Mean WBA_{TPP} for the control group showed two large peaks with the first peak occurring at 1.25–1.5 kHz and the second peak at 3 kHz. In comparison, mean WBA_{TPP} of the OME group showed a large peak at 2.5 kHz. Mean WBA_{TPP} of the OME group was lower than that of the 25th percentile of the control group at all frequencies between 0.4 and 6 kHz. On the other hand, mean WBA_{TPP} of the control group was above the 75th percentile of the OME group at all frequencies except 8 kHz (→ **Figure 2B**).

In the control group, both mean WBA_A and WBA_{TPP} were the highest between 1 and 4 kHz and reduced <1 kHz and >4 kHz (→ **Figure 3A**). These findings were consistent with the results of several studies that have reported absorbance to vary across

frequencies in children (Beers et al⁶; Ellison et al⁸). The frequency region between 1 and 4 kHz is the most sensitive frequency region for middle ear assessments as energy is transmitted most efficiently through the middle ear. Hence, any change in middle ear transmission due to middle ear dysfunction can easily be detected in this region. Studies by Keefe et al,²⁶ Ellison et al⁸ and Sanford and Brockett⁴¹ demonstrated that absorbance at frequencies between 1 and 4 kHz provided good discriminability of middle ear function in children.

The main aim of the present study was to compare the predictive accuracy of WBA_A and WBA_{TPP} to detect OME in children. The present study showed that both WBA_A and WBA_{TPP} identified OME with high accuracy. The frequency region between 1 and 2.5 kHz had the highest accuracy (AROC ≥ 0.80) for WBA_A , whereas the frequency region between 0.6 and 2.5 kHz had the highest accuracy for WBA_{TPP} . Optimal test performance for WBA_A was achieved at 1.5 kHz with an AROC of 0.92 and sensitivity and specificity of 0.92. In comparison, optimal test performance for WBA_{TPP} was obtained at 1.25 kHz with an AROC of 0.91, sensitivity of 0.88, and specificity of 0.94. Overall, WBA_{TPP} showed predictive accuracy across a wider frequency region (0.3–6 kHz) with better sensitivity than WBA_A (0.6–4 kHz). The AROC for WBA_{TPP} was significantly greater than that for WBA_A at 0.3, 0.4, and 0.6 kHz. These results suggest that WBA_{TPP} can provide additional and diagnostically useful information across a wider frequency region than WBA_A .

In comparison, several studies have investigated the predictive accuracy of WBA_A in identifying OME in children (Ellison et al⁸; Keefe et al²⁶; Terzi et al⁵³). Terzi et al⁵³ compared WBA_A in healthy children and children diagnosed with OME during myringotomy. They reported that WBA_A had high diagnostic values at 1 and 1.5 kHz with an AROC of 0.973 and 0.967, respectively. Ellison et al⁸ reported an AROC of 0.93 for a univariate measure of WBA_A determined across frequencies 0.25–8 kHz. Beers et al⁶ compared WBA_A in children with normal middle ear status and children with OME confirmed through pneumatic otoscopy and video otomicroscopy. They reported high diagnostic accuracy with AROC between 0.95 and 0.97 at 1–4 kHz. The highest accuracy of 0.97 was observed at 1.2 and 1.6 kHz. However, the present study showed an AROC of 0.90 at 1.25 kHz and 0.92 at 1.5 kHz for WBA_A , 0.90 at 0.8 kHz and 1 kHz, and 0.91 at 1.25 kHz for WBA_{TPP} . Although the present study demonstrated that both WBA_A and WBA_{TPP} could predict OME in children with high accuracy, they were slightly lower when compared with that of the above studies. The discrepancies could be due to the use of different subject samples and methods.

The present study also evaluated the diagnostic accuracy of 226-Hz tympanometry against surgical findings as the gold standard. The results showed high predictive accuracy with an AROC of 0.93 (95% CI: 0.88–0.99). These results are comparable with the optimal test performance of WBA_A at 1.5 kHz (AROC 0.92; 95% CI: 0.86–0.97) and WBA_{TPP} at 1.25 kHz (AROC 0.91; 95% CI: 0.83–0.98). However, these results are not consistent with those obtained by Beers et al⁶ who noted that the AROC of

WBA_A at 1.25 kHz (AROC 0.97; 95% CI: 0.94–0.99) was greater than that of 226-Hz tympanometry using Y_{tm} (AROC 0.81; 95% CI: 0.75–0.87). Similarly, Keefe et al²⁶ reported that both WBA_A and tympanometric WBA tests were better predictors of conductive hearing loss (AROC values ≥ 0.97) than 226-Hz tympanometry using tympanometric width as the dependent variable (AROC ranging from 0.68 to 0.93). Furthermore, they found no significant difference in AROC between WBA_A and tympanometric WBA. Terzi et al⁵³ also reported WBA_A to be more accurate than 226-Hz tympanometry using qualitative measures of classifying tympanograms.

The main reason for the difference between the present study and the aforementioned studies could be due to the fact that dry ears were not included in the present study, whereas the studies by Keefe et al²⁶ and Beers et al⁶ might have included dry ears as there was no surgical confirmation of middle ear effusions. Another reason could be due to ceiling effect where all three tests are equally effective in identifying ears with definite effusion, whereas they may perform differently when there is a varying degree of difficulties in separating ears with OME from normal ears.

Ellison et al⁸ investigated the test performance of WBA_A to detect OME and reported an AROC of 0.93 (95% CI: 0.87–0.97). They also measured admittance magnitude (AROC: 0.93; 95% CI: 0.87–0.97), phase angle (AROC: 0.90; 95% CI: 0.82–0.95), and combined predictor of all three measures (AROC: 0.94; 95% CI: 0.88–0.98) and noted no significant differences between them. However, Ellison et al⁸ used pneumatic otoscopy results as the reference standard and concluded that WBA_A measures are at least as effective in predicting the presence of fluid in OME cases as those methods currently recommended by clinical guidelines which includes pneumatic otoscopy and 226-Hz tympanometry.

WBA_A and WBA_{TPP} with different tympanometric patterns (normal, negative middle ear pressure and flat) obtained with the OME group was analyzed. In total, 52 ears had flat tympanograms, six ears had negative middle ear pressure and two ears had normal tympanograms in the OME group. As illustrated in **Figure 4**, in general, for all the tympanogram types, both mean WBA_A and WBA_{TPP} were reduced from 0.25 to 0.5 kHz. Between 0.5 and 2.5 kHz, OME ears with normal tympanogram had the largest mean WBA_A and WBA_{TPP} with values approaching the control group and slightly better than the control group at 1.25 and 1.5 kHz and decreasing steeply >2.5 kHz for mean WBA_{TPP}.

In comparison, ears with flat tympanograms in the OME group showed the lowest absorbance for both mean WBA_A and WBA_{TPP}. OME ears with negative middle ear pressure showed absorbance in between OME with normal and flat tympanograms. OME ears with negative middle ear pressure and normal tympanogram demonstrated improvement in mean WBA_{TPP} relative to mean WBA_A from 0.5 to 2.5 kHz and reduced absorbance >2.5 kHz. Despite the small number of ears with negative middle ear pressure, WBA_{TPP} provides useful data for ears with pre-existing middle ear pathology and negative middle ear pressure. WBA_{TPP} measure compensates for the effect of the difference in pressure between the ear canal and the middle ear. For example, when child has

a middle ear condition (fluid in the middle ear) plus Eustachian tube dysfunction (significant negative pressure), the WBA_{TPP} results will be significantly reduced when compared with control group even after compensating for the pressure differences. This may indicate presence of a pre-existing pathological condition (OME) in addition to Eustachian tube dysfunction as suggested by Margolis et al.³²

Mean WBA_A of children in the control and OME groups was compared with the previously reported studies by Keefe et al²⁶ and Terzi et al.⁵³ **Figure 5** shows the comparison of mean WBA_A with control and OME groups of present study with other studies. Apart from slight differences in the WBA_A, the results of the present study were comparable with those reported by the earlier studies. Results of control and OME group in the present study resembled closely to Keefe et al²⁶ study, whereas results of the study by Terzi et al⁵³ showed improved absorbance for the control group ~ 1 –2 kHz and OME group ~ 1.5 –3 kHz. Mean WBA_A in healthy ears were highest between 2 and 4 kHz and reduced <2 and >4 kHz. Mean WBA_A was reduced in ears with OME across all frequencies when compared with healthy ears.

The present study also analyzed the absorbance result based on thickness of the middle ear fluid as determined by an experienced ENT surgeon. Although classification of middle ear fluid was subjective, it revealed interesting findings. Both thick and thin fluid demonstrated similar absorbance pattern for WBA_A with thin fluid showing slightly better absorbance between 0.8 and 2.5 kHz, and between 3 and 6 kHz. However, under WBA_{TPP} condition, thin fluid showed higher absorbance across the frequency range from 0.25 to 8 kHz, suggesting that WBA_{TPP} may have the ability to identify the thickness and/or viscosity of the middle ear fluid.

Several researchers have suggested that considering WBA over a frequency band is better than WBA at individual frequencies (Hunter et al¹⁹; Ellison et al⁸; Terzi et al⁵³). For instance, Hunter et al¹⁹ proposed area indices and they reported that absorbance in the frequency ranges ~ 2 kHz (e.g., 1–2, 1–4, 2–4 kHz) provided the best prediction of referring on distortion product otoacoustic emissions in neonates. Terzi et al⁵³ investigated the efficiency of WBA_A in identifying OME in children and reported that WBA averaged from 0.375 to 2 kHz had the highest diagnostic value of 0.984. Ellison et al⁸ combined the multivariate information across frequencies into a univariate predictor and reported an AROC of 0.93 for WBA_A for diagnosing OME. The present study showed an AROC of 0.92 for averaged WBA_A between 1 and 2 kHz, 0.91 for averaged between 0.3–2 kHz and 0.90 for averaged between 2 and 8 kHz. These values agree with the above studies that have demonstrated high AROC for WBA_A averaged over a frequency band. Nevertheless, AROC averaged across 1–2 kHz for WBA_A was the same as AROC obtained at 1.5 kHz. However, AROC averaged across 1–2 kHz for WBA_{TPP} (0.88) was less than AROC at individual frequencies of 0.8, 1, and 1.25 kHz (**Table 4**).

Implications of the Study

The high test performance of WBA_A and WBA_{TPP} against myringotomy suggests that both measures have high predictive accuracy for identification of OME in children. However,

WBA_{TPP} showed predictive accuracy across a wider frequency range (0.3–6 kHz) than WBA_A (0.6–4 kHz). In addition to this, WBA_{TPP} provides useful data for ears with both fluid and negative middle ear pressure conditions indicating that WBA_{TPP} can provide additional and diagnostically useful information such as reduced absorbance even after compensating for the pressure differences (Aithal et al¹).

There was no significant difference in the predictive accuracy of WBA_A and WBA_{TPP} when compared with 226-Hz admittance tympanometry and neither test performed significantly better than the other in identifying ears with definite effusion as confirmed by surgery. However, in clinical situations, WBA and 226-Hz admittance tympanometry may perform differently when there are varying degrees of OME.

The result of the present study also suggests that apart from individual frequencies, WBA_A and WBA_{TPP} in the frequency band between 0.3 and 2 kHz, 1 and 2 kHz, and 2 and 8 kHz may identify the presence of OME in children. The cutoff values of 1–2 kHz averaged mean absorbance values of 0.38 and 0.51 for WBA_A and WBA_{TPP}, respectively, in the present study (► **Table 4**) may suggest the presence of OME in children. Cutoff values for other frequency bands are provided in the ► **Table 4**.

The result of the present study also suggests that WBA_{TPP} may have the ability to classify the middle ear fluid as thick or thin noninvasively and may become a useful clinical tool to predict the nature of the middle ear fluid preoperatively. However, a large-scale study with objective methods of classifying middle ear fluid along with other wideband immittance measures is needed to confirm this observation.

Limitations of the Study

The loose age criterion for inclusion of children in the OME group could have confounded the results in the present study. Because of small sample size under different age group, effect of age was not studied in this study. The 10th percentile cutoff WBA_A and WBA_{TPP} values were based on the normative values for the control group with an age range of 4.11–11.4 years and applied to the OME group where the age ranged from 1.1 to 14.3 years. Keefe et al²⁴ have shown that developments of the conductive system that strongly affect the acoustic responses of the ear are not complete at 24 months of age. Therefore, it is important to develop age-specific criteria for WBA_A and WBA_{TPP} for the determination of OME in younger children.

Another limitation of the study is that compensation was not done for the residual positive pressure during the probe insertion. This could have an impact on the results as the residual positive pressure due to probe insertion could potentially be different in both the control and OME group. Furthermore, WAI measures of admittance, phase angle, equivalent ear canal volume, and resonance frequency were not analyzed in this study. It is possible that these measurements may provide distinctive profiles that might be useful for discrimination of different middle ear pathologies as suggested by Sanford and Brockett⁴¹ and may be useful in separating dry ears from ears with fluids in OME cases.

Conclusions

Both WBA_A and WBA_{TPP} demonstrated high test performance in predicting OME, but neither test performed significantly better than the other or 226-Hz admittance tympanometry. WBA_{TPP} showed predictive accuracy across a wider frequency region than WBA_A. The AROC for WBA_A was highest (0.92) at 1.5 kHz, whereas the AROC for WBA_{TPP} was highest (0.91) at 1.25 kHz.

Abbreviations

AC	air conduction
ANOVA	analysis of variance
AROC	area under ROC
BC	bone conduction
CI	confidence intervals
ENT	ear nose and throat
IQR	interquartile range
OME	otitis media with effusion
ROC	receiver operating characteristics
TEOAEs	transient evoked otoacoustic emissions
TPP	tympanometric peak pressure
WAI	wideband acoustic immittance
WBA	wideband absorbance
WBA _A	wideband absorbance measured at ambient pressure
WBA _{TPP}	wideband absorbance measured at tympanometric peak pressure
WBT	wideband tympanometry

Conflict of Interest

None declared.

References

- 1 Aithal S, Aithal V, Kei J, Anderson S, Liebenberg S. Eustachian tube dysfunction and wideband absorbance measurements at tympanometric peak pressure and 0 daPa. *J Am Acad Audiol* 2019; 30:781–791
- 2 Aithal S, Kei J, Driscoll C. Wideband reflectance in young infants (0-6 months): a cross-sectional study. *J Am Acad Audiol* 2014; 25:471–478
- 3 Aithal S, Kei J, Driscoll C, Khan A. Normative wideband reflectance measures in healthy neonates. *Int J Pediatr Otorhinolaryngol* 2013;77:29–35
- 4 Aithal S, Yonovitz A, Aithal V. Perceptual consequences of conductive hearing loss: speech perception in indigenous students learning English as a 'school' language. *Aust N Z J Audiol* 2008; 30:1–18
- 5 Aithal V, Yonovitz A, Aithal S. Tonal masking level differences in Aboriginal children: implications for binaural interaction, auditory processing disorders and education. *Aust N Z J Audiol* 2006; 28:31–40
- 6 Beers AN, Shahnaz N, Westerberg BD, Kozak FK. Wideband reflectance in normal Caucasian and Chinese school-aged children and in children with otitis media with effusion. *Ear Hear* 2010;31:221–233
- 7 Bess FH. Hearing loss associated with middle ear effusion: workshop on effects of otitis media on the child. *Pediatrics* 1983; 71:640–641

- 8 Ellison JC, Gorga MA, Cohn E, Fitzpatrick DF, Sanford CA, Keefe DH. Wideband acoustic transfer functions predict middle-ear effusion. *Laryngoscope* 2012;122:887–894
- 9 Finitzo T, Friel-Patti S, Chinn K, Orval B. Tympanometry and otoscopy prior to myringotomy: issues in diagnosis of otitis media. *Int J Pediatr Otorhinolaryngol* 1992;24:101–110
- 10 Fria TJ, Cantekin EI, Eichler JA. Hearing acuity of children with otitis media with effusion. *Arch Otolaryngol* 1985; 111:10–16
- 11 Friel-Patti S, Finitzo T. Language learning in a prospective study of otitis media with effusion in the first two years of life. *J Speech Lang Hear Res* 1990;33:188–194
- 12 Graydon K, Rance G, Dowell R, Van Dun B. Consequences of early conductive hearing loss on long-term binaural processing. *Ear Hear* 2017;38:621–627
- 13 Greenhouse SW, Geisser S. On the methods in the analysis of profile data. *Psychometrika* 1959;24:95–112
- 14 Groon KA, Rasetshwane DM, Kopun JG, Gorga MP, Neely ST. Air-leak effects on ear-canal acoustic absorbance. *Ear Hear* 2015; 36:155–163
- 15 Hall JW, Grose JH, Pillsbury HC. Long-term effects of chronic otitis media on binaural hearing in children. *Arch Otolaryngol Head Neck Surg* 1995;121:847–852
- 16 Hanley JA, McNeil BJ. The meaning and use of the area under a receiver operating characteristic (ROC) curve. *Radiology* 1982; 143:29–36
- 17 Harris PK, Hutchinson KM, Moravec J. The use of tympanometry and pneumatic otoscopy for predicting middle ear disease. *Am J Audiol* 2005;14:3–13
- 18 Hunter LL, Bagger-Sjoberg D, Lundberg M. Wideband reflectance associated with otitis media in infants and children with cleft palate. *Int J Audiol* 2008;47(1, Suppl):S57–S61
- 19 Hunter LL, Feeney MP, Miller JAL, Jeng PS, Bohning S. Wideband reflectance in newborns: normative regions and relationship to hearing-screening results. *Ear Hear* 2010;31:599–610
- 20 Hunter LL, Margolis RH, Giebink GS. Identification of hearing loss in children with otitis media. *Ann Otol Rhinol Laryngol* 1994; 103:59–61
- 21 Hunter LL, Tubaugh L, Jackson A, Propes S. Wideband middle ear power measurement in infants and children. *J Am Acad Audiol* 2008;19:309–324
- 22 Jeng PS, Levitt H, Lee WW, Gravel JS. Reflectance measures for detecting otitis media with effusion in children: Preliminary findings, Proceedings of the 7th International Symposium on Recent Advances in Otitis Media with Effusion. Ft. Lauderdale, FL: BC Decker Inc; 2002:194–199
- 23 Keefe DH, Archer KL, Schmid KK, Fitzpatrick DF, Feeney MP, Hunter LL. Identifying otosclerosis with aural acoustical tests of absorbance, group delay, acoustic reflex threshold, and otoacoustic emissions. *J Am Acad Audiol* 2017;28: 838–860
- 24 Keefe DH, Bulen JC, Arehart KH, Burns EM. Ear-canal impedance and reflection coefficient in human infants and adults. *J Acoust Soc Am* 1993;94:2617–2638
- 25 Keefe DH, Gorga MP, Neely ST, Zhao F, Vohr B. Ear-canal acoustic admittance and reflectance measurements in human neonates. II. Predictions of middle-ear dysfunction and sensorineural hearing loss. *J Acoust Soc Am* 2003;113:407–422
- 26 Keefe DH, Sanford CA, Ellison JC, Fitzpatrick DF, Gorga MA. Wideband aural acoustic absorbance predicts conductive hearing loss in children. *Int J Audiol* 2012;51:880–891
- 27 Keefe DH, Simmons JL. Energy transmittance predicts conductive hearing loss in older children and adults. *J Acoust Soc Am* 2003; 114:3217–3238
- 28 Kei J, Allison-Levick J, Dockray J, Harrys R, Kirkegard C, Wong J, Maurer M, Hegarty J, Young J, Tudehope D. High-frequency (1000 Hz) tympanometry in normal neonates. *J Am Acad Audiol* 2003;14:20–28
- 29 Keogh T, Kei J, McMahon S. Speech perception abilities of children with and without histories of recurrent otitis media: an overview. *Asia Pac J Speech Lang Hear* 2004;9:1–7
- 30 Klausen O, Moller P, Holmeffjord A, Reisaeter S, Asbjornsen A. Lasting effects of otitis media with effusion on language skills and listening performance. *Acta Otolaryngol Suppl* 2000;543:73–76
- 31 Lildholdt T. Negative middle ear pressure: variations by season and sex. *Ann Otol Rhinol Laryngol* 1980;89:67–70
- 32 Margolis RH, Saly GL, Keefe DH. Wideband reflectance tympanometry in normal adults. *J Acoust Soc Am* 1999;106:265–280
- 33 Margolis RH, Saly GL, Hunter LL. High-frequency hearing loss and wideband middle ear impedance in children with otitis media histories. *Ear Hear* 2000;21:206–211
- 34 Northern JL, Downs MP. *Hearing in Children*. 4th ed. Baltimore, MD: Williams and Wilkins; 1991
- 35 Nozza RJ, Bluestone CD, Kardtzke D, Bachman KR. Towards the validation of aural acoustic immittance measures for diagnosis of middle ear effusion in children. *Ear Hear* 1992;13:442–453
- 36 Nozza RJ, Bluestone CD, Kardtzke D, Bachman KR. Identification of middle ear effusion by aural acoustic immittance measures for diagnosis of middle ear effusion in children. *Ear Hear* 1994; 15:310–323
- 37 Palmu A, Puhakka H, Rahko T, Takala AK. Diagnostic value of tympanometry in infants in clinical practice. *Int J Pediatr Otorhinolaryngol* 1999;49:207–213
- 38 Paradise JL, Feldman HM, Campbell TF, Dollaghan CA, Rockette HE, Pitcairn DL, Smith CG, Colborn DK, Bernard BS, Kurs-Lasky M, Janosky JE, Sabo DL, O'Connor RE, Pelham WE Jr. Tympanostomy tubes and developmental outcomes at 9 to 11 years of age. *N Engl J Med* 2007;356:248–261
- 39 Roberts J, Wallace IF. Language and otitis media. In: Roberts J, Wallace IF, eds. *Otitis Media in Young Children*. Baltimore, MD: Brookes; 1997
- 40 Rosenfeld RM, Culpepper L, Doyle KJ, Grundfast KM, Hoberman A, Kenna MA, Lieberthal AS, Mahoney M, Wahl RA, Woods CR Jr, Yawn B; American Academy of Pediatrics Subcommittee on Otitis Media with Effusion; American Academy of Family Physicians; American Academy of Otolaryngology-Head and Neck Surgery. Clinical practice guideline: otitis media with effusion. *Otolaryngol Head Neck Surg* 2004;130(5, Suppl):S95–S118
- 41 Sanford CA, Brockett JE. Characteristics of wideband acoustic immittance in patients with middle ear dysfunction. *J Am Acad Audiol* 2014;25:425–440
- 42 Sanford CA, Feeney MP. Effects of maturation on tympanometric wideband acoustic transfer functions in human infants. *J Acoust Soc Am* 2008;124:2106–2122
- 43 Sanford CA, Keefe DH, Liu Y-W, Fitzpatrick DF, McCreery RW, Lewis DE, Gorga MP. Sound-conduction effects on distortion-product otoacoustic emission screening outcomes in newborn infants: test performance of wideband acoustic transfer functions and 1-kHz tympanometry. *Ear Hear* 2009;30:635–652
- 44 Shahnaz N, Bork K. Wideband reflectance norms for Caucasian and Chinese young adults. *Ear Hear* 2006;27:774–788
- 45 Shahnaz N, Bork K, Polka L, Longridge N, Bell D, Westerberg BD. Energy reflectance and tympanometry in normal and otosclerotic ears. *Ear Hear* 2009;30:219–233
- 46 Shahnaz N, Feeney MP, Schairer KS. Wideband acoustic immittance normative data: Ethnicity, gender, aging, and instrumentation. *Ear Hear* 2013;34:27s–35s
- 47 Shanks JE, Shelton C. Basic principles and clinical applications of tympanometry. *Otolaryngol Clin North Am* 1991;24:299–328
- 48 Shaffer AD, Ford MD, Choi SS, Jabbar N. The impact of tympanostomy tubes on speech and language development in children with cleft palate. *Otolaryngol Head Neck Surg* 2017;157:504–514
- 49 Shekelle P, Takata G, Chan LS, Mangione-Smith R, Corley PM, Mophew T, Morton S. *Diagnosis, Natural History and Late Effects of Otitis Media with Effusion*. Rockville, MD: Agency for Healthcare Research and Quality; 2003

- 50 Stool SE, Berg AO, Berman S. Otitis Media with Effusion in Young Children. Clinical Practice Guideline No. 12 Guideline for OME. Rockville, MD: National Institute of Health, US Department of Health and Human Services; 1994
- 51 Takata GS, Chan LS, Morphew T, Mangione-Smith R, Morton CS, Shekelle P. Evidence assessment of the accuracy of methods of diagnosing middle ear effusion in children with otitis media with effusion. *Pediatrics* 2003;112:1379–1387
- 52 Teele DW, Klein JO, Chase C, Menyuk P, Rosner BA. Otitis media in infancy and intellectual ability, school achievement, speech, and language at age 7 years. *J Infect Dis* 1990;162:685–694
- 53 Terzi S, Ozgur A, Erdivanli OC, Coskun Z, Ogurlu M, Demirci M, Dursun E. Diagnostic value of the wideband acoustic absorbance test in middle-ear effusion. *J Laryngol Otol* 2015;129:1078–1084
- 54 Valente M, Fernandez E, Monroe H. *Audiology Answers for Otolaryngologists*. New York, NY: Thieme; 2011
- 55 Vander Werff KR, Prieve BA, Georgantas LM. Test-retest reliability of wideband reflectance measures in infants under screening and diagnostic test conditions. *Ear Hear* 2007;28:669–681
- 56 Wallace IF, McCarton CM, Bernstein R, Gravel JS, Stapells D, Ruben RJ. Otitis media, auditory sensitivity, and language outcomes at one year. *Laryngoscope* 1988;98:64–70
- 57 Watters GW, Jones JE, Freeland AP. The predictive value of tympanometry in the diagnosis of middle ear effusion. *Clin Otolaryngol Allied Sci* 1997;22:343–345
- 58 Winiger AM, Alexander JM, Diefendorf AO. Minimal hearing loss: from a failure-based approach to evidence-based practice. *Am J Audiol* 2016;25:232–245
- 59 Yonovitz L, Yonovitz A, Nienhuys TG, Boswell J. MLD evidence of auditory processing factors as a possible barrier to literacy for Australian Aboriginal children. *Aust J Educ Deaf* 1995;1:34–42